



HOKKAIDO UNIVERSITY

Title	Determination of Cu, Pb, Cd and Zn in Seawater by Anodic Stripping Voltammetry
Author(s)	Abe, Kazuo; 阿部, 和雄; Matsunaga, Katsuhiko et al.
Citation	北海道大學水産學部研究彙報, 34(4), 350-354
Issue Date	1983-12
Doc URL	https://hdl.handle.net/2115/23839
Type	departmental bulletin paper
File Information	34(4)_P350-354.pdf



Determination of Cu, Pb, Cd and Zn in Seawater by Anodic Stripping Voltammetry

KAZUO ABE*, KATSUHIKO MATSUNAGA*, KOHJI IGARASHI*,
ISAO KUDO* and SHIGERU FUKASE*

Abstract

Analytical conditions to determine considerably low concentrations of heavy metals in seawater by anodic stripping voltammetry were examined. This method can prevent a sample from becoming contaminated by metals, and also determine the metals with small amount of a sample. The precision of Cu, Pb, Cd and Zn, of which the concentrations are 50, 40, 30 and 700 ng/l, were 27, 22, 19 and 11 % respectively.

Introduction

As to the concentration of heavy metals in seawater, recently reported values have been decreased by factors of one-tenth to one-hundredth (Boyle & Edmond, 1975; Sclater et al., 1976; Boyle et al., 1976; Moor & Burton, 1976; Moor, 1978; Bruland et al., 1978-a, 1978-b; Danielsson, 1978; Bruland, 1980; Knauer & Martin, 1981; Schaule & Patterson, 1981; Heggie, 1982). The reason for this is assumed to be the development of new sampling bottles to prevent samples from being contaminated by metals, and of highly sensitive analytical instruments. With the development of the highly sensitive analytical instruments, it has been possible to detect the metals that have been contaminated by a sampler or a storage bottle. For studying the biochemical or geochemical cycles of the metals, it is important to determine the reliable concentration of the metals in seawater.

Analytical techniques are broadly divided into flameless atomic absorption spectrophotometry (FAAS) and anodic stripping voltammetry (ASV). The former is widely used by many investigators and the latter only by Heggie (1982), Spencer et al. (1982) and Batley (1983).

As FAAS is not so sensitive, the metals must be concentrated from large amounts of samples. It is very difficult to do this, however, without the metals becoming contaminated. On the other hand, ASV is highly sensitive, so the metals can be determined by using small amounts of samples.

In this paper, an analytical method for determining the metals in seawater by ASV is described.

* *Laboratory of Marine Chemistry, Faculty of Fisheries, Hokkaido University*
(北海道大学水産学部海洋科学講座)

Experiment

Apparatus and reagents

A Yanako P-1000 Voltammetric Analyzer was used with a hanging mercury drop electrode (Metrohm EA 290), a platinum wire electrode and a saturated calomel electrode as a reference electrode. A polarogram was recorded by a Watanabe X-Y recorder.

Mercury and water were purified using a vacuum distiller and a quartz glass distiller respectively. Deoxygenation was carried out with highly pure nitrogen gas.

Procedure

Transfer 40 ml of a sample solution to an electrolysis cell, and deoxygenate with nitrogen gas for 20 min with stirring. Preelectrolyse the metals at -1.3 V for 15 min (1 min for Zn) with stirring at 400 rpm. Stop stirring and allow to stand for 20 sec. Scan the electrode potential from -1.3 to 0.0 V at a scan rate of 20 mV/sec with a 50 mV pulse amplitude and record the polarogram. Determine the concentration of Cu, Pb, Cd and Zn by the standard addition method.

Analytical conditions

Analytical conditions were examined with a solution containing a concentration of 500 ng/l in seawater of each metal.

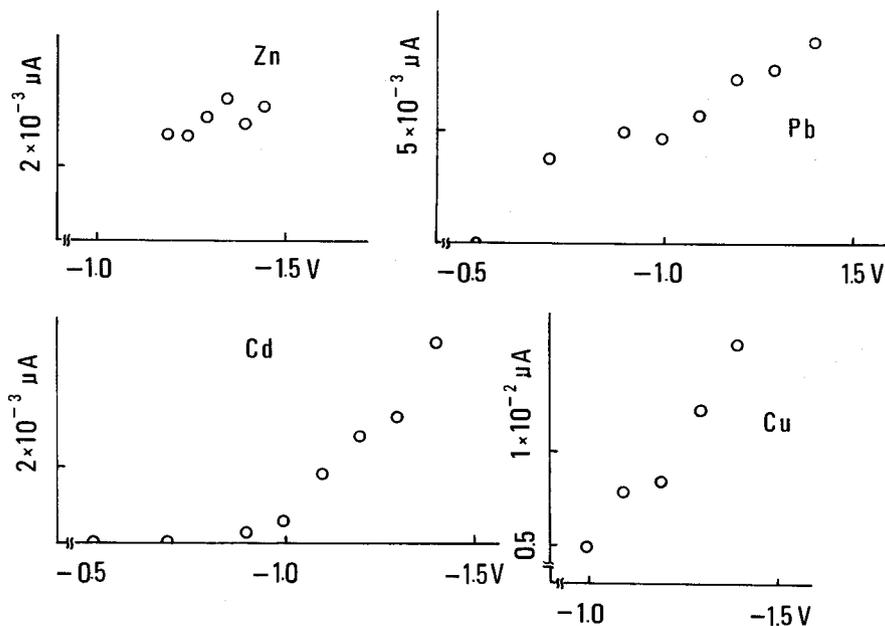


Fig. 1. Effect of preelectrolysis potential on peak current

Effect of preelectrolysis potential on peak current

All peak currents of the metals increased with rising potential in the negative direction (Fig. 1). However, the reduction of the hydrogen ion began at about -1.5 V and disturbed the peak currents of the metals. Therefore, the most favorable preelectrolysis potential was -1.3 V.

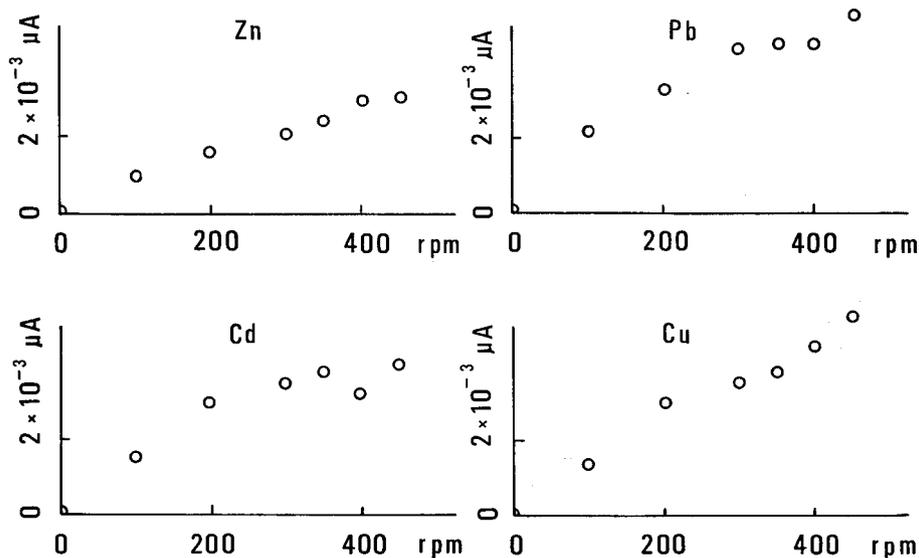


Fig. 2. Effect of stirring rate on peak current

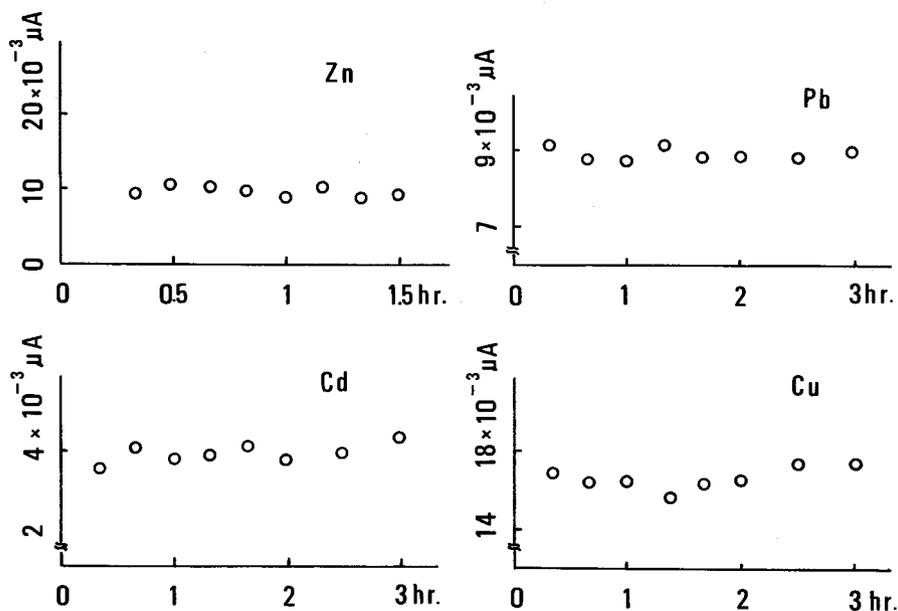


Fig. 3. Adsorption of the metals on the walls of an electrolysis cell

Table 1. Precision for Zn

	Zn(ng/l)
1. $y=0.0145 X+11.3$	782
2. $y=0.6158 X+11.0$	697
3. $y=0.0163 X+12.9$	791
4. $y=0.0163 X+10.8$	662
5. $y=0.0165 X+11.0$	666
Slope	$\mu=0.0158\pm 0.0010$ 6.4% ($\alpha=0.05$)
Concentration	$\mu=716\pm 78$ (ng/l) 11% ($\alpha=0.05$)

Table 2. Precision for Cd

	Cd(ng/l)
1. $y=0.110 x+2.83$	25.4
2. $y=0.093 x+3.30$	35.5
3. $y=0.102 x+2.70$	26.3
4. $y=0.100 x+2.60$	25.9
5. $y=0.112 x+3.00$	26.7
Slope	$\mu=0.103\pm 0.0097$ 9.4% ($\alpha=0.05$)
Concentration	$\mu=27.9\pm 5.3$ (ng/l) 19% ($\alpha=0.05$)

Table 3. Precision for Pb

	Pb(ng/l)
1. $y=0.0408 x+1.61$	39.0
2. $y=0.0356 x+1.60$	44.8
3. $y=0.0397 x+2.00$	50.3
4. $y=0.0335 x+1.80$	46.7
5. $y=0.0422 x+1.52$	30.7
Slope	$\mu=0.0394\pm 0.0032$ 8.2% ($\alpha=0.05$)
Concentration	$\mu=42.3\pm 9.5$ (ng/l) 22% ($\alpha=0.05$)

Table 4. Precision for Cu

	Cu(ng/l)
1. $y=0.0435 x+2.04$	46.8
2. $y=0.0463 x+3.40$	73.4
3. $y=0.0495 x+3.20$	64.5
4. $y=0.0483 x+2.60$	53.7
5. $y=0.0516 x+2.20$	56.1
Slope	$\mu=0.0478\pm 0.0038$ 8.0% ($\alpha=0.05$)
Concentration	$\mu=56.1\pm 14.9$ (ng/l) 26% ($\alpha=0.05$)

Effect of stirring rate on peak current

The peak currents of the metals increased as the stirring rate increased (Fig. 2). It was difficult, however, to hold a mercury drop on the hanging mercury drop electrode at a stirring rate of more than 500 rpm.

Adsorption of the metals on the walls of an electrolysis cell

A sample was allowed to stand in the cell for several hours to test the adsorption of the metals in the sample on the walls. As shown in Fig. 3, it was found that the metals did not adsorb on the walls within 3 hr.

Precision

The reproducibility of the method was determined by addition of the metals to seawater. The concentration of each metal was determined from an intercept of a working curve.

The relative standard deviations of the concentration of each, and the slopes of the working curves for 5 replicate determinations, are shown in Tables 1-4.

References

- Batley, G.E. (1983): Electroanalytical techniques for the determination of heavy metals in seawater. *Mar. Chem.* **12**, 107-117.
- Boyle, E. and J.M. Edmond (1975): Copper in surface waters of south of New Zealand. *Nature* **253**, 107-109.
- Boyle, E.A., F. Selater and J.M. Edmond (1976): On the marine geochemistry of cadmium.

Ibid 263, 42-44.

- Bruland, K.W., G.A. Knauer and J.H. Martin (1978a): Cadmium in northeast Pacific waters. *Limnol. Oceanogr.* 23, 618-625.
- Bruland, K.W., G.A. Knauer and J.H. Martin (1978b): Zinc in northeast Pacific water. *Earth Planet. Sci. Lett.* 47, 176-198.
- Bruland, K.W. (1980): Oceanographic distribution of cadmium, zinc, nickel and copper in the north Pacific. Ibid 47, 176-198.
- Danielsson, L.G. (1980): Cadmium, cobalt, iron, lead nickel and zinc in Indian Ocean water. *Mar. Chem.* 8, 199-215.
- Heggie, D.T. (1982): Copper in surface waters of the Bering Sea. *Geochim. Cosmochim. Acta* 46, 1031-1036.
- Knauer, G.A. and J.H. Martin (1981): Phosphorus-cadmium cycling in northeast Pacific waters. *J. Mar. Res.* 39, 65-76.
- Moore, R.M. and J.D. Burton (1976): Concentration of dissolved copper in the eastern Atlantic Ocean 23°N to 47°N. *Nature* 264, 241-243.
- Moore, R.M. (1978): The distribution of dissolved copper in the eastern Atlantic Ocean. *Earth Planet. Sci. Lett.* 41, 461-468.
- Schaule, B.K. and C.C. Patterson (1981): Lead concentrations in the northeast Pacific: evidence for global anthropogenic perturbations. Ibid 54, 97-116.
- Selater, F.R., E. Boyle and J.M. Edmond (1976): On the marine geochemistry of nickel. *Ibid* 31, 119-128.
- Spencer, M.J., P.R. Betzer and S.R. Piotrowicz (1982): Concentrations of cadmium, copper, lead and zinc in surface waters of the northwest Atlantic Ocean—a comparison of Go-flow and teflon water sampler. *Mar. Chem.* 11, 403-410.