



HOKKAIDO UNIVERSITY

Title	Predictors and Proarrhythmic Consequences of Inappropriate Implantable Cardioverter-Defibrillator Therapy
Author(s)	Tenma, Taro; Yokoshiki, Hisashi; Mizukami, Kazuya et al.
Citation	Circulation Journal, 79(9), 1920-1927 https://doi.org/10.1253/circj.CJ-15-0306
Issue Date	2015-08-25
Doc URL	https://hdl.handle.net/2115/71892
Type	journal article
File Information	79_CJ-15-0306_1.pdf, Supplementary File: Figure S1



Predictors and Proarrhythmic Consequences of Inappropriate Implantable Cardioverter-Defibrillator Therapy

Taro Tenma, MD; Hisashi Yokoshiki, MD, PhD; Kazuya Mizukami, MD; Hirofumi Mitsuyama, MD, PhD; Masaya Watanabe, MD, PhD; Ryo Sasaki; Motoki Maeno; Yoshiro Matsui, MD, PhD; Hiroyuki Tsutsui, MD, PhD

Supplementary File 1

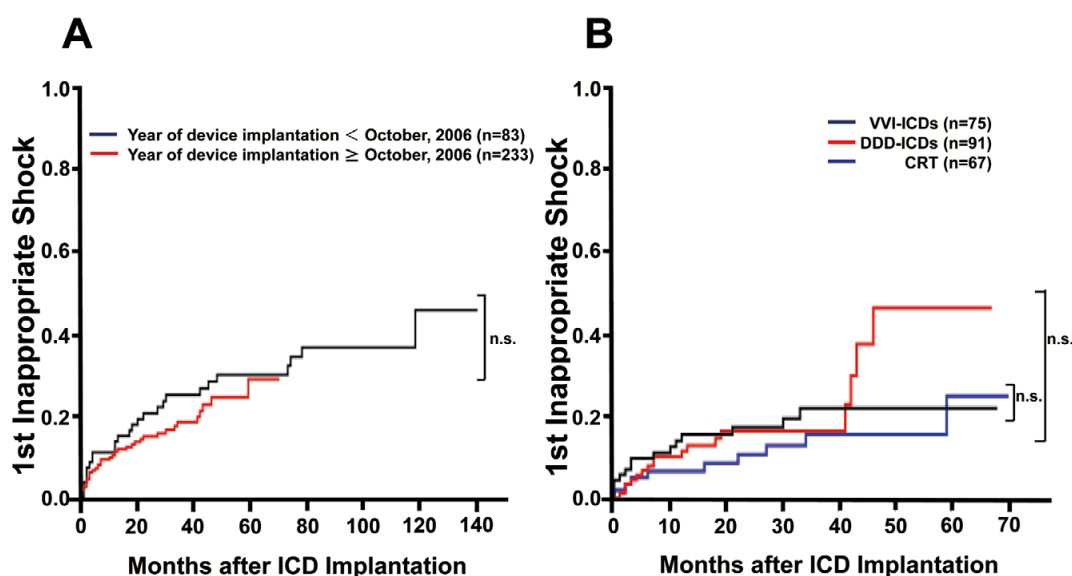


Figure S1. Cumulative event rate for first inappropriate shock comparing period of ICD implantation and device type. **(A)** Kaplan-Meier curve demonstrates the occurrence of first inappropriate shock in patients who received their ICD before (black line) and after (red line) October 2006. **(B)** Kaplan-Meier curve shows the incidence of inappropriate shocks among patients with single-chamber (VVI) ICDs, dual-chamber (DDD) ICDs, and biventricular ICDs for cardiac resynchronization therapy (CRT) in the “recent” (year of device implantation after October 2006) group (n=233). ICD, implantable cardioverter-defibrillator.