HOKKAIDO UNIVERSITY

Title	Mechanical effect of an implant under denture base in implant-supported distal free-end removable partial dentures
Author(s)	村島, 直道
Degree Grantor	北海道大学
Degree Name	博士(歯学)
Dissertation Number	甲第13856号
Issue Date	2020-03-25
DOI	https://doi.org/10.14943/doctoral.k13856
Doc URL	https://hdl.handle.net/2115/78199
Type	doctoral thesis
File Information	Naomichi_Murashima.pdf

Hokkaido University Collection of Scholarly and Academic Papers : HUSCAP

博 士 論 文

Mechanical effect of an implant under denture base
in implant-supported distal free-end removable partial dentures
（インプラントに支持を求めた遊離端部分床義歯におけるインプラントの力学的効果）

令和２年３月申請

北海道大学
大学院歯学研究科口腔医学専攻

村 島 直 道

Introduction

Removable partial dentures (RPDs) are generally used for recovery of oral function of partially edentulous patients. However, RPDs occasionally cause many problems such as insufficient recovery of function, overload of abutment teeth, and resorption of residual ridge [1,2].

Recently, dental implants (hereinafter abbreviated simply as “implants”) are widely used and recommended as one of the best options than RPDs for partial edentulism, due to their masticatory function and satisfaction of patients [3]. However, they demand amount / quality of bone and are accompanied with surgical invasion [4].

On the other hand, implant assisted RPDs (IARPDs) are clinically used and reported as a better option of prosthodontic treatment for higher satisfaction of patients [5,6]. Furthermore, applicability of shorter implants can decrease surgical invasion and expand indication [7,8]. However, their mechanical advantage is not clear [9-19].

The aim of this study was therefore to investigate the influence of an implant under the saddle of distal extended removable partial dentures on stress sharing among abutment teeth and residual ridge, using finite element (FE) models based on CT images.

Materials and methods

FE models

This study used CT data of a patient with defect of mandibular right molars in the Department of Removable Prosthodontics, Hokkaido University Hospital. Outline of bone and teeth were extracted from the CT images encoded in Digital Imaging and Communications in Medicine (DICOM) format according to the CT value by computer-aided design (CAD) software [Materialise Mimics Medical 21.0 (Materialise, Leuven, Belgium)]. FE model of the right half of the mandible, teeth, implant, and a denture was constructed and analyzed as a bilateral distal free-end removable partial denture (Fig. 1).

The outline of PDL and mucosa was constructed with a Computer Added Design (CAD) software (Materialise 3-matics Medical 12.0, Materiarise, Leuven, Belgium) from the surface of teeth and alveolar residual bone, respectively. Metal frameworks of RPD and IARPDs was designed with denture frame CAD software (DIGISTELL, C4W/DIGILEA, France) (fig. 2). The Co-Cr framework had a set of a cingulum rest, an I-bar clasp, and a distal proximal plate on each abutment tooth (Fig. 3).

Cylindrical dental implant made by titanium, with 3.5mm in diameter and 8.5mm in width was placed under denture saddle. Their location was region of first premolar, second premolar or first molar (IARPD4, IARPD5 and IARPD6, respectively). In addition, a model without an implant (RPD) was constructed as a control. These CAD

data were outputted as Standard Triangulated Language (STL) files.

The CAD data were imported into FEA pre-post processor software (Marc. Mentat2010, MSC USA) and converted into FE models (Fig. 4). Material properties indicated Table 1. This study was approved by the Institutional Review Board of Hokkaido University Hospital for Clinical Research (016-0152).

Condition of contact

Condition of contact at the interfaces of mucosa-denture base, denture base- implant, and retainer-abutment tooth was considered in the analysis. Friction at these interfaces without the retainer-tooth interface were neglected, according to the lubricate effect of saliva. The coefficient of friction at the retainers was determined as μ=0.05 [20-22].

Boundary conditions

In IARPD models (IARPD4, IARPD5 and IARPD6), we decided amount of relief between the top of the implant and the denture base so that they are in contact with each other under 100N of vertical load on L6 (Table 2) [24,25].

The displacement was restricted at each node on the top of condyle and the stop of masseter muscle for all direction, and at all nodes in cross section of the midline of mandible for lateral direction (Fig. 5).

Vertical load of 200N was applied on one of the loading points located on the point corresponding to first premolar (L4), second premolar (L5), and first molar tooth (L6) and second molar tooth (L7). (Fig. 6).

Evaluation of the analysis

We evaluated each model with the relative vertical displacement of denture base at its distal end and apex of abutment tooth (canine) with reference to the nearest node on the surface of bone. We also evaluated the distribution of equivalent stress in alveolar ridge.

Results

Equivalent stress in alveolar mucosa (Fig. 7-10).

In all models, the stress was largest under the L7 load, compared with the other load conditions. IARPD6 showed most effective reduction of stress by placing an implant compared with RPD.

Likewise, the amount of the displacement of denture base was the largest under L7 load (Fig.11). As the position of an implant was more distally located, the displacement decreased proportionally.

Equivalent stress in PDL (Fig. 12-15).

The RPD model showed a decrease of the stress in PDL under L7 load compared to the L4, L5, and L6 loads. However, the IARPD models showed the most decrease under L6 load. Compared with RPD, most of all IARPD models shows reduction of stress in PDL, except for IARPD5 under L7 load.

Fig. 16 showed vertical displacement at the apex of canine. In the RPD model, the vertical displacement of canine became smaller as the loading point located distally. On the other hand, in all of the IARPD models, the canine displaced upward under L7 load.

Discussion

In the free-end denture, the masticatory efficiency decreases because the denture sinks and the stress on the abutment tooth increases accordingly [29-32]. Therefore, clinical application by IARPD has been proposed [5,6].

There are several reports concerned with the mechanical behavior of the abutment teeth and implants of IARPDs under occlusal load [11,14]. Moreover, FE models generated from computed Tomography (CT) images becomes common recently. However, there are only a few reports on stress analysis with precise FE models of IARPDs based on CT images, because of the complexity of shapes, material properties, and boundary conditions including contact analysis [12,15,16,18]

In this study, FE analysis was performed with rough elements for the implant and bone

to reduce analysis time within the limit by the hardware used since the purpose of this study is to investigate the burden of the abutment tooth and mucosa. Therefore, the occlusal pressure burden of the implant and the surrounding bone could not be evaluated in this study. In order to evaluate the distribution of stress in implants and surrounding bones under IARPDs, it is necessary to construct models with preciseshape of the implant and surrounding bone including the thread.

The amount of relief was determined so that the top of the implant would be in contact with denture base under occlusal force during mastication of about 100N. Since the displacement of the mucosa is much larger than that of the implant, the behavior of the denture base under occlusal force smaller than 100N was basically the same as that of conventional RPDs [24,25]. Therefore, if the relief was small, the implant would contact under smaller occlusal force and support most of occlusal force like one of a fixed prosthesis. On the contrary, too much relief would result in the same behavior of denture base as conventional RPDs unless a stronger occlusal force is applied.

With respect to the location of an implant, more distally location was favorable because of effective reduction of stress in mucosa and PDL of abutment teeth. However, more distally located load than the implant lifted abutment teeth. This displacement was due to the lever effect with a fulcrum of implant. However, in IARPD4 model, this effect was

negligible because of the smallest movement of denture base around the implant, which was near the rest of the retainer on canine.

Matsudate described that there were cases where lifting to the abutment tooth occurs in the model study on unilateral free-end cases [14].

The results of this study also correspond with the report by Ohyama et al [17]. They described that the implant under denture base reduced displacement of abutment teeth under load located mesially, because it suppressed the displacement of denture base in unilateral free-end IARPDs.

On the other hand, from this study, it seemed to be better to locate an implant in the second molar area because it was speculated that the displacement of denture base and abutment teeth can be suppressed more effectively than IARPD6. However, it was impossible to place an implant there in the case used this study because of insufficient bone height from mandibular canal. Although shorter implant would be applicable, its effect on IARPDs should be investigated in the future.

Conclusion

Within the limitations of this study, the area corresponding to the first molar was recommended for the location of an implant under denture base of bilateral distal free-

end IARPDs. The implant located in the area corresponding to second premolar can cause non-physiological extrusion force on abutment teeth by the load on the artificial second molar.

Acknowledgments

The author is grateful to Keigo Nishikawa and Mitsuru Sakano in Medical Dental Laboratory, Hokkaido university hospital for their assistance with metal framework design. The author also thanks Michinori Matsumoto and Taichi Ishihara in SDL/HD Co. Ltd for lending their expertise on CAD software.

References

[1] Bert TC, Kamal A, Edward D. Removable partial denture abutment tooth movement as affected by inclination of residual ridges and type of loading. J Prosthet Dent 1971; 25(4): 375

[2] Qiufei X, Timo ON, Juha MN, Juhani W, Anja A. Oral status and prosthetic factors related to residual ridge resorption in elderly subjects. Acta Odontologica Scandinavica 1997; 55(5): 306-313

[3] Krishan KK. Veterans-Administration cooperative dental implant study-comparisons between fixed partial dentures supported by blade-vent implants and removable partial dentures. Part IV comparisons of patient satisfaction between 2 treatment modalities. J Prosthet Dent 1991; 66(4):517-530

[4] Daniel B, Karl D, Daniel H, Hans P, Urs CB. Localized ridge augmentation with autografts and barrier membranes. Periodontol 2000 1999; 19: 151-63

[5] Ohkubo C, Kobayashi M, Suzuki Y, Hosoi T. Effect of Implant Support on Distal-Extension Removable Partial Dentures: In Vivo assessment. Int J Oral Maxillofac Implants 2008; 23(6): 1095-1101

[6] De Kok IJ, Chang KH, Lu TS, Cooper LF. Comparison of Three-Implant-Supported Fixed Dentures and Two-Implant-Retained Overdentures in the Edentulous Mandible: A Pilot Study of Treatment Efficacy and Patient Satisfaction. Int J Oral Maxillofac Implants 2011; 26(2): 415-426

[7] Bakke M, Holm B, Holm, B. Masticatory Function and Patient Satisfaction with Implant-Supported Mandibular Overdentures: A Prospective 5-Year Study. Int J Prosthodont 2002; 15(6): 575-581

[8] Mijiritsky E, Lorean A, Mazor Z, Levin L. Implant Tooth-Supported Removable Partial Denture with at Least 15-Year Long-Term Follow-Up. Clin Implant Dent Relat Res 2015; 17(5): 917-922

[9] Ligia Del' Arco Pignatta Cunha. Evaluation of the Influence of Location of Osseointegrated Implants Associated with Mandibular Removable Partial Dentures. Implant Dent 2008; 17(3): 278-287

[10] Verri FR, Pellizzer EP, Pereira JA, Zuim PR, Santiago Júnior JF. Evaluation of Bone Insertion Level of Support Teeth in Class I Mandibular Removable Partial Denture Associated with an Osseointegrated Implant: A Study Using Finite Element Analysis. Implant Dent 2011; 20(3): 192-201

[11] Sato M, Suzuki Y, Kurihara D, Shimpo H, Ohkubo C. Effect of implant support on mandibular distal extension removable partial dentures: Relationship between denture supporting area and stress distribution. J prosthodont Res 2013; 57(2): 109-112

[12] Shahmiri R, Aarts JM, Bennani V, Atieh MA, Swain MV. Finite Element Analysis of an Implant-assisted Removable Partial Denture. J Prosthodont 2013; 22(7): 550-555

[13] Memari Y, Geramy A, Fayaz A, Rezvani Habib Abadi S, Mansouri Y. Influence of Implant Position on Stress Distribution in Implant-Assisted Distal Extension Removable Partial Dentures: A 3D Finite Element Analysis: J Dent (Tehran) 2014;11(5): 523-30

[14] Matsudate Y, Yoda N, Nanba M, Ogawa T, Sasaki K. Load distribution on abutment tooth, implant and residual ridge with distal-extension implant-supported removable partial denture. J prosthodont Res 2016; 60(4): 282-288

[15] Xiao W, Li Z, Shen S, Chen S, Chen S, Wang J. Influence of connection type on the biomechanical behavior of distal extension mandibular removable partial dentures supported by implants and natural teeth. Comput Methods Biomech Biomed Engin 2016; 19(3): 240-247

[16] Eom JW, Lim YJ, Kim MJ, Kwon HB. Three-dimensional finite element analysis of implant-assisted removable partial dentures. J Prosthet Dent 2017; 117(6): 735-742

[17] Ohyama T, Nakabayashi S, Yasuda H, Kase T, Namaki S. Mechanical analysis of the effects of implant position and abutment height on implant-assisted removable partial dentures. J Prosthodont Res 2019; 9(45): 30355-30360

[18] Liu Y, Zhang YN, Sasaki K, Chen XD. Influence of location of osseointegrated implant on stress distribution in implant supported longitudinal removable partial dentures: 3-dimensional finite element analysis. Int J Clin Exp Med 2019; 12(8):10399-10410

[19] Ortiz-Puigpelat O, Lázaro-Abdulkarim A, de Medrano-Reñé JM, Gargallo-Albiol J, Cabratosa-Termes J, Hernández-Alfaro F. Influence of Implant Position in Implant-Assisted Removable Partial Denture: A Three-Dimensional Finite Element Analysis. J Prosthodont 2019;28: e675-e681

[20] Muraki H, Wakabayashi N, Park I, Ohyama T. Finite element contact stress analysis of the RPD abutment tooth and periodontal ligament. J Dent 2004; 32(8); 659-665

[21] Sato Y, Abe Y, Yuasa Y Akagawa Y. Effect of friction coefficient on Akers clasp retention. J Prosthet dent 1997; 78(1): 22-27

[22] Ohida M, Yoda K, Nomura N, Hanawa T, Igarashi Y. Evaluation of the static frictional coefficients of Co-Cr and gold alloys for cone crown telescope denture retainer applications. Dent Mater J 2010; 29(6): 706-712

[23] Korioth TW, Hannam AG. Deformation of the human mandible during simulated tooth clenching. J Dent Res 1994; 73(1): 56-66

[24] Kumagai H, Suzuki T, Hamada T, Sondang P, Fujitani M, Nikawa H. Occlusal force distribution on the dental arch during various levels of clenching. J Oral Rehabilitation 1999; 26(12): 932-935

[25] Kasai K, Takayama Y, Yokoyama A. Distribution of Occlusal Forces During Occlusal Adjustment of Dental Implant Prostheses: A Nonlinear Finite Element Analysis Considering the Capacity for Displacement of Opposing Teeth and Implants. Int J Oral Maxillofac implants 2012; 27(2): 329-335

[26] Lytle RB. Soft Tissue Displacement Beneath Removable Partial and Complete Dentures. J Pros Dent 1962; 12(1): 34-43

[27] Monteith BD. Management of loading forces on mandibular distal-extension prostheses. Part I: Evaluation of concepts for design. J Prosthet Dent 1984; 52(5): 673-681

[28] Kunavisarut C, Lang LA, Stoner BR, Felton DA. Finite element analysis on dental implant-supported prostheses without passive fit. J Prosthodont 2002; 11(1): 30-40

[29] Cecconi BT, Asgar K, Dootz E. Removable partial denture abutment tooth movement as affected by inclination of residual ridges and type of loading. J Prosth Dent 1971; 25(4): 375-381

[30] Wills DJ, Manderson RD. Biomechanical aspects of the support of partial dentures. J Dent 1977; 5(4): 310-318

[31] Craig RG, Farah JW. Stress from loading distal-extension removable partial dentures. J Prosthet Dent 1978; 39(3): 274-277

[32] Monteith BD. Management of loading forces on mandibular distal-extension prostheses. Part I: Evaluation of concepts for design. J Prosthet Dent 1984; 52(5): 673-681

Table 1. Material properties [23, 26-28]

		Elastic modulus（MPa）	Poison’s ratio
Bone (coronal bone)		13700	0.30
Mucosa		0.5	0.45
Tooth	Enamel	80000	0.30
	Dentin	17600	0.25
Co-Cr alloy		211000	0.3
Denture (Acrylic resin)		2200	0.31
Titanium		110000	0.33
PDL		2.3	0.49

Table 2. Relief amount of between implant and denture on 100N vertical load

	IARPD4	IARPD5	IARPD6
Relief amount (mm)	0.06122	0.09335	0.12698

Fig. 1 CT date (DICOM) of mandibula bone

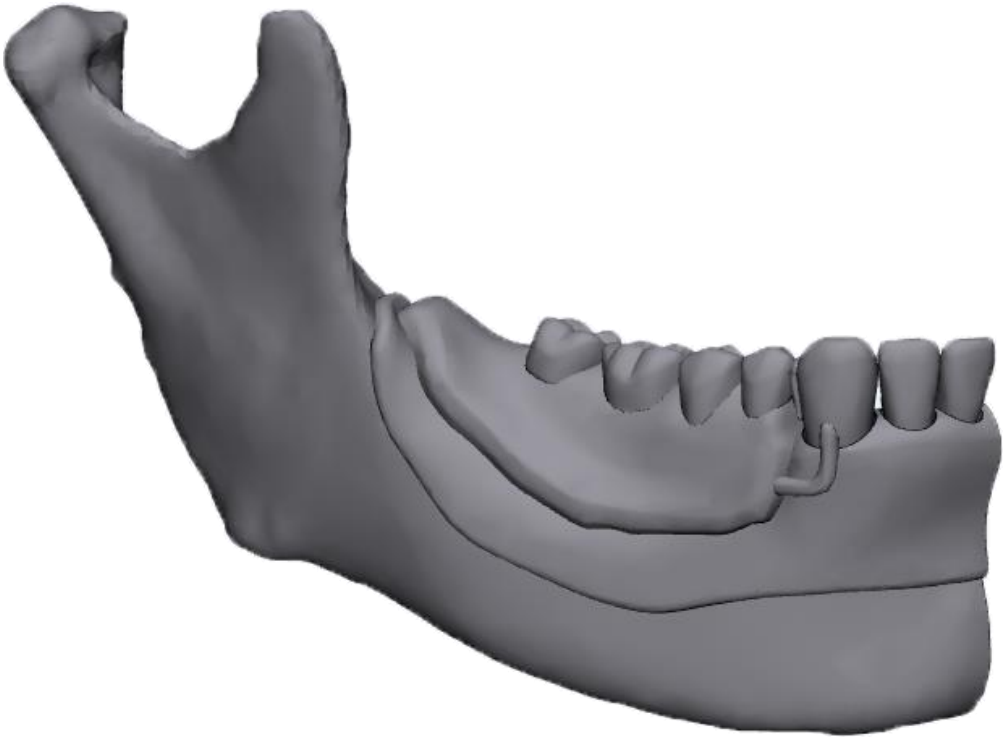

Fig. 2 CAD model (STL format)

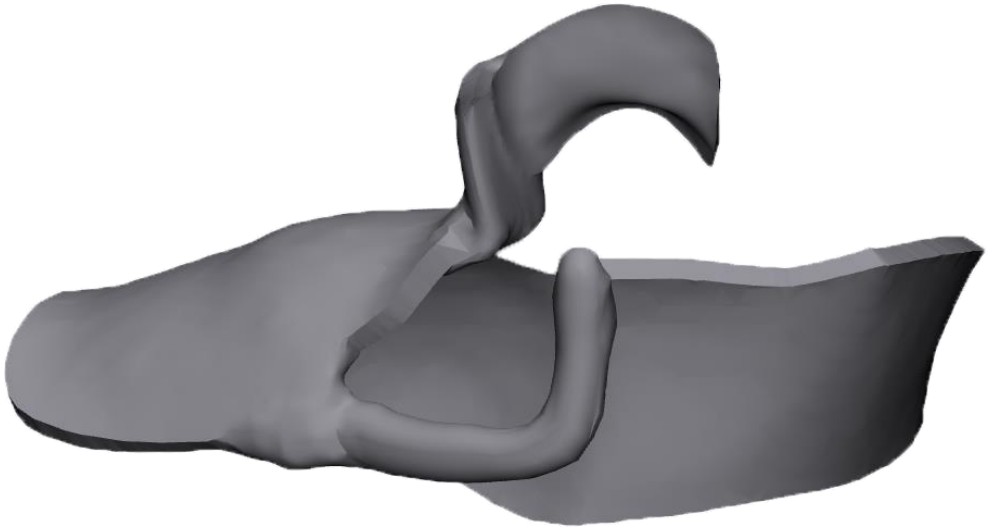

Fig. 3. Denture Metal frame was designed with denture frame CAD software (DIGISTELL, C4W/DIGILEA, France) and imported with CAD software (3-matics 12.0). The Co-Cr framework had a set of a cingulum rest, an I-bar clasp, and a distal proximal plate on each abutment tooth.

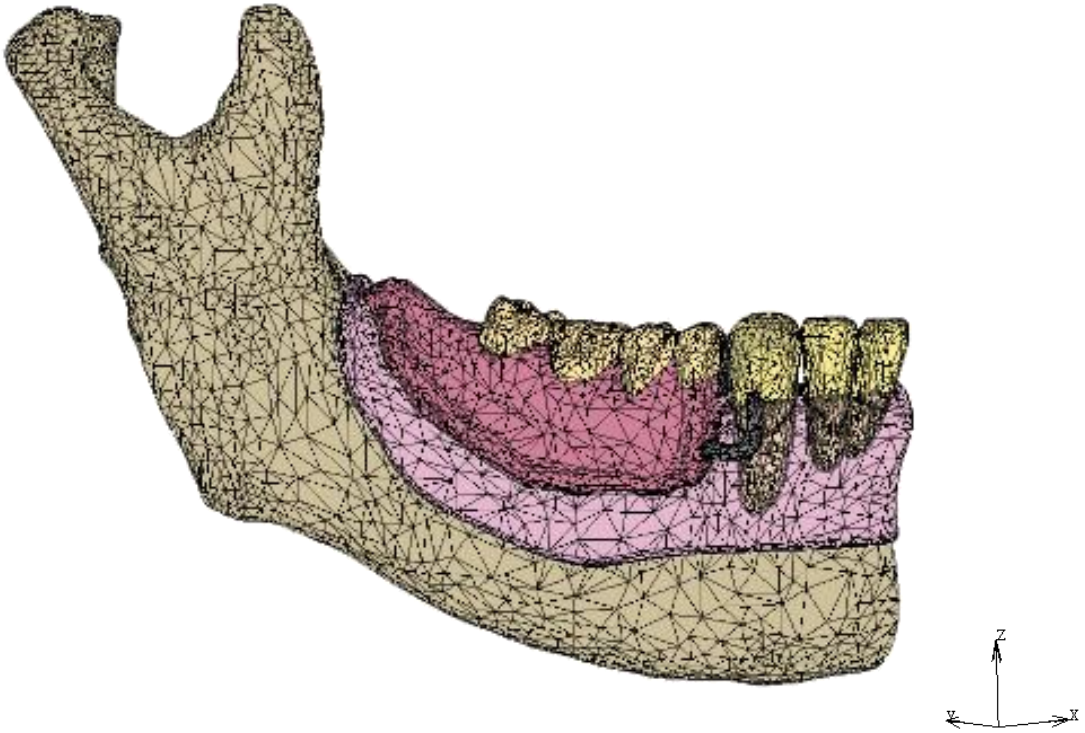

Fig. 4 Bilateral distal free-end removable partial denture FE model. Material properties are displayed in table 1. [15-18]. All materials were assumed to be isotropic and elastic.

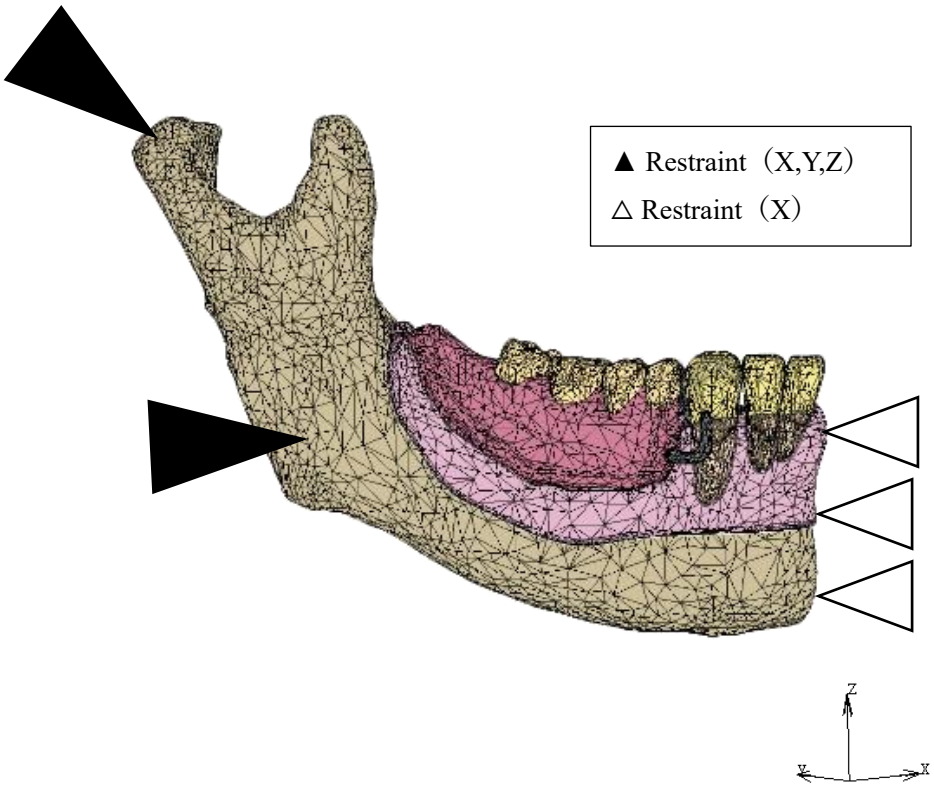

Fig. 5 Boundary condition

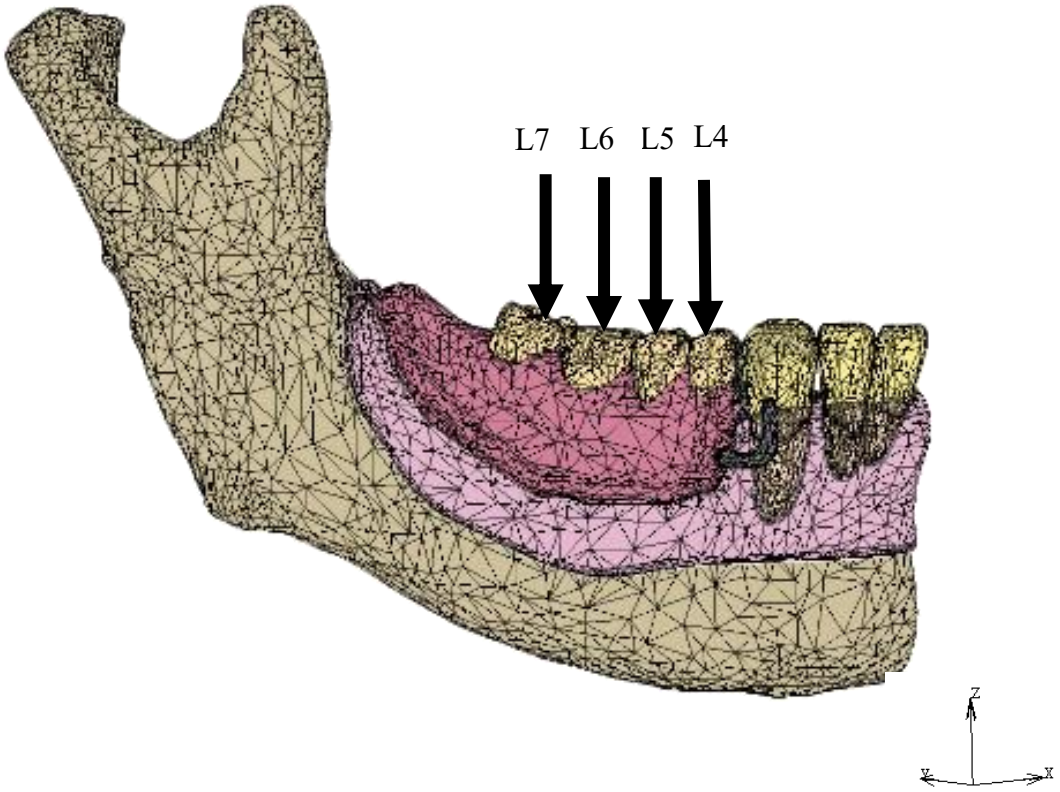

Fig. 6 Load point

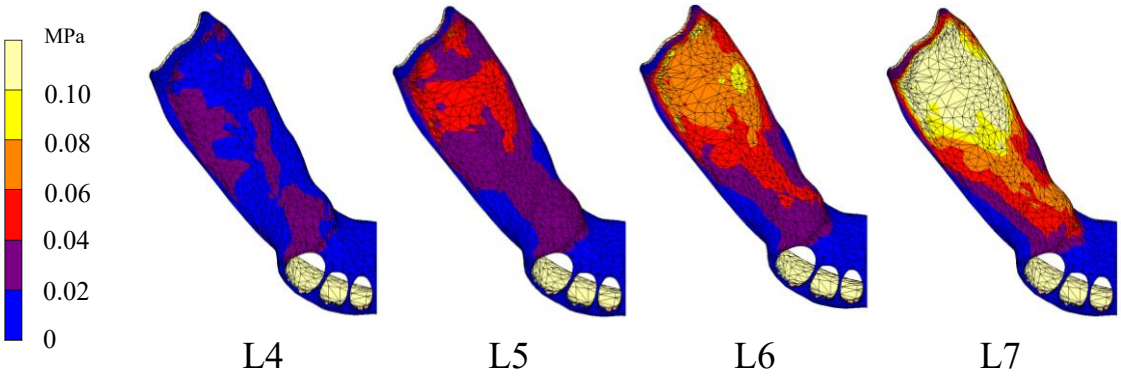

Fig. 7 Equivalent stress of mucosa area (RPD)

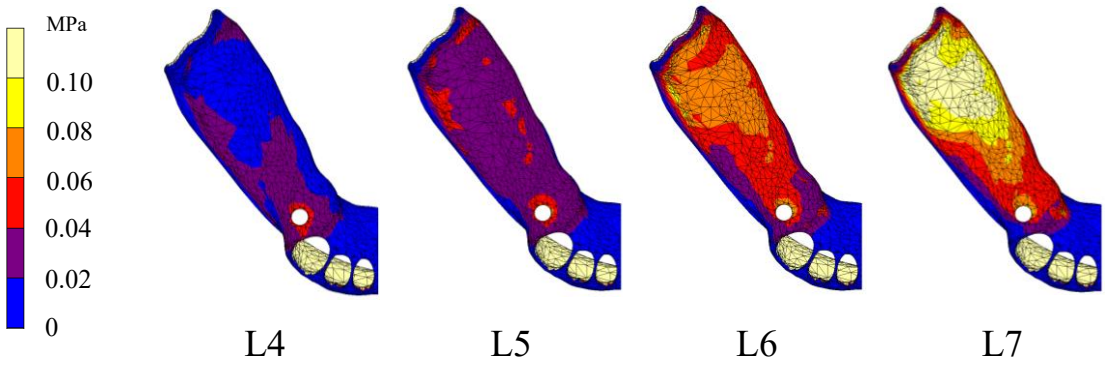

Fig. 8 Equivalent stress of mucosa area (IARPD4)

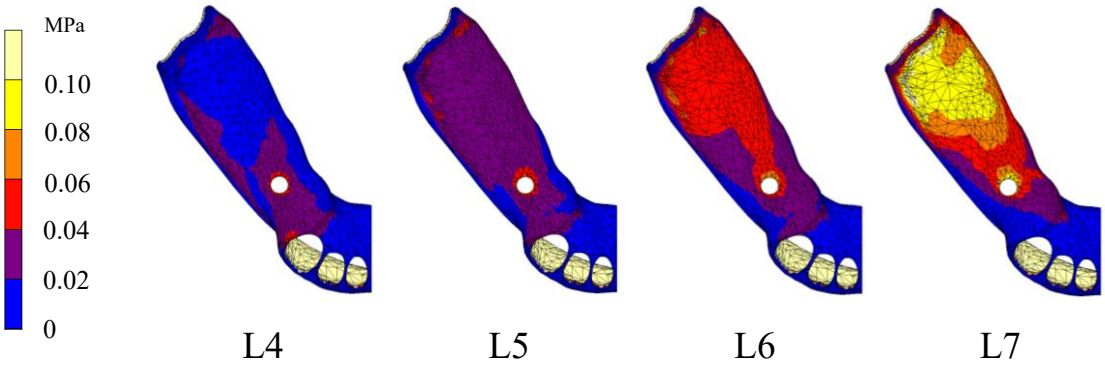

Fig. 9 Equivalent stress mucosa area (IARPD5)

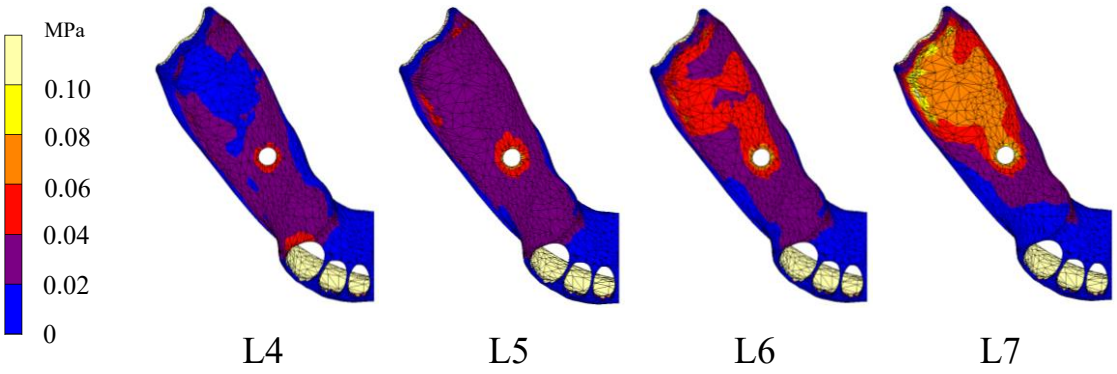

Fig. 10 Equivalent stress of mucosa area (IARPD6)

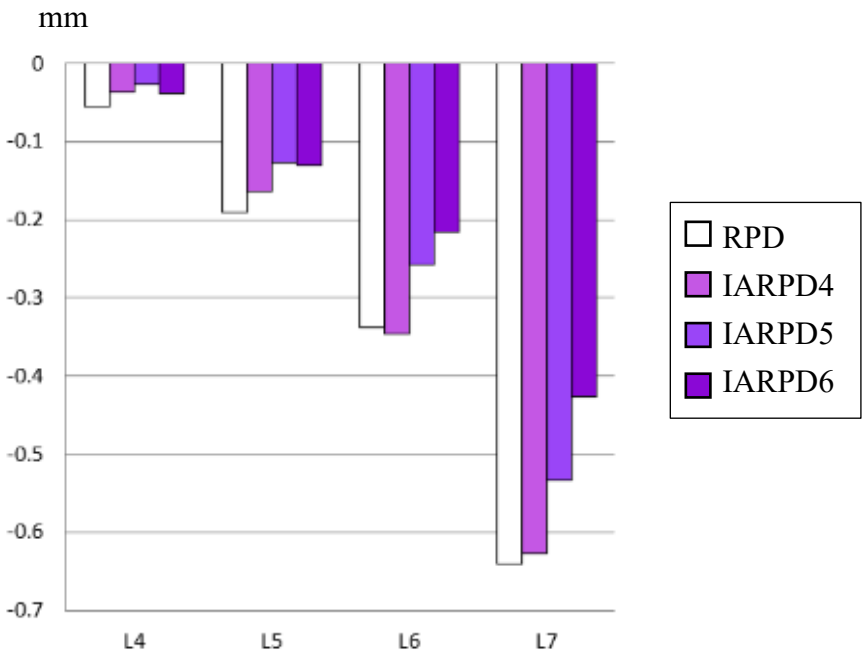

Fig. 11 Displacement of denture

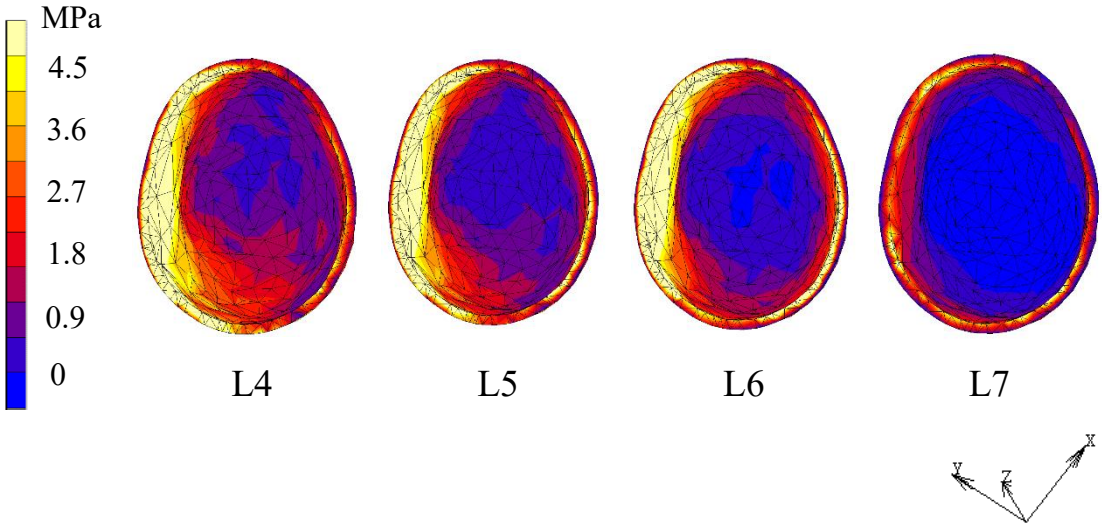

Fig. 12 Equivalent stress of canine PDL (RPD)

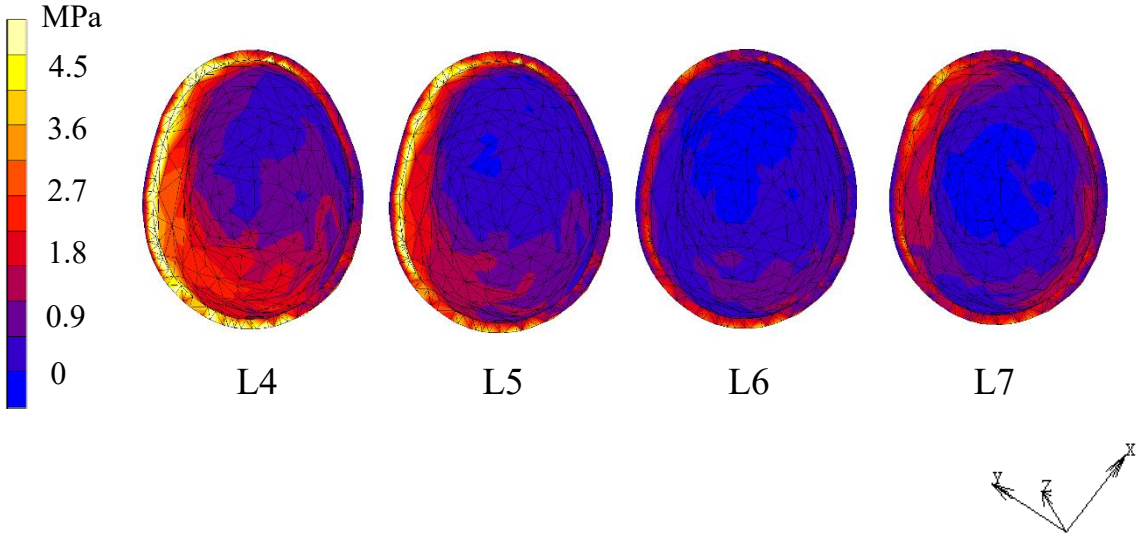

Fig. 13 Equivalent stress of canine PDL (IARPD4)

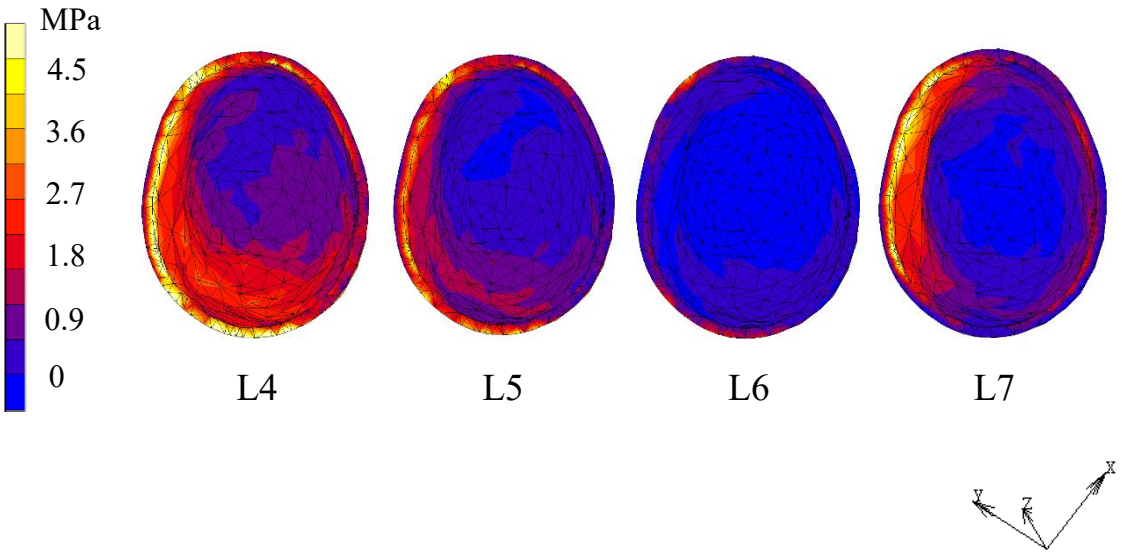

Fig. 14 Equivalent stress of canine PDL (IARPD5)



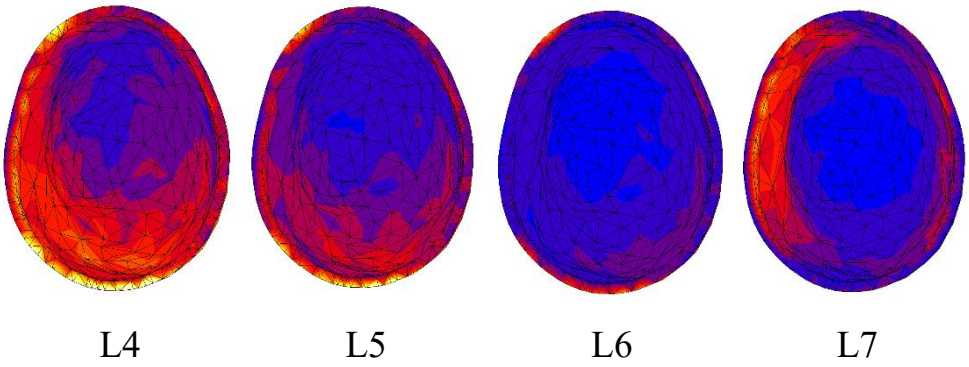

Fig. 15 Equivalent stress of canine PDL (IARPD6)

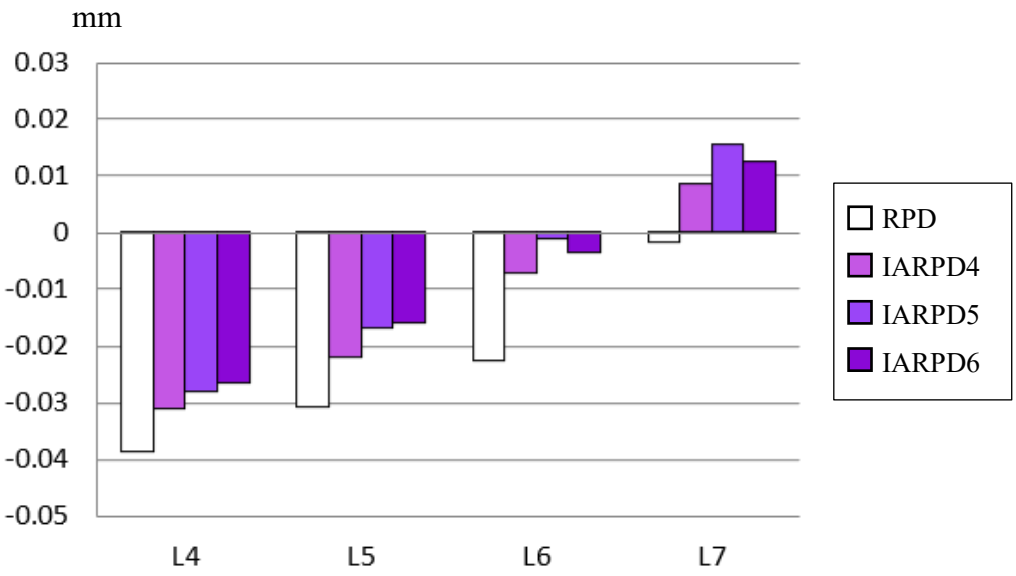

Fig. 16 Displacement of canine apex area