



HOKKAIDO UNIVERSITY

Title	Improvement of nerve imaging speed with coherent anti-Stokes Raman scattering rigid endoscope using deep-learning noise reduction
Author(s)	Yamato, Naoki; Niioka, Hirohiko; Miyake, Jun et al.
Citation	Scientific Reports, 10(1), 15212 https://doi.org/10.1038/s41598-020-72241-x
Issue Date	2020-09-16
Doc URL	https://hdl.handle.net/2115/79383
Rights(URL)	https://creativecommons.org/licenses/by/4.0/
Type	journal article
File Information	41598_2020_72241_MOESM1_ESM.pdf, Supplementary information



Improvement of nerve imaging speed with coherent anti-Stokes Raman scattering rigid endoscope using deep-learning noise reduction

Naoki Yamato, Hirohiko Niioka, Jun Miyake and Mamoru Hashimoto

Supplementary information

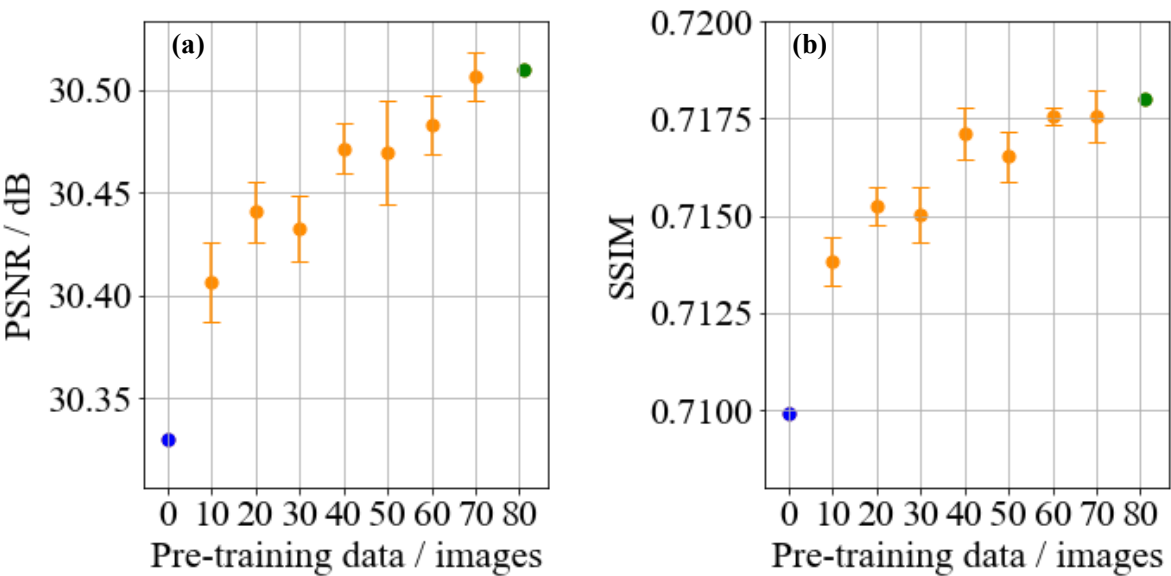


Figure S1 Results of N2N with fine-tuning for the amount of pre-training images of CARS microscopy. The metrics for test images of CARS endoscopy at 12.5 images/min (exposure time of 4.8 seconds) are shown. The blue plots are the results of N2N with endoscopy, the green plots are N2N with fine-tuning shown in Table 2. The amount of pre-training images of CARS microscopy was changed from 10 to 70 (step: 10). The pre-training images at each amount were randomly selected from 81 images 5 times. Each plot from 10 to 70 shows the average and standard deviation of 5 results. As the pre-training images increase, both evaluation metrics are improved.