



HOKKAIDO UNIVERSITY

| | |
|------------------|---|
| Title | Tele-assessment of bandwidth limitation for remote robotics surgery |
| Author(s) | Ebihara, Yuma; Oki, Eiji; Hirano, Satoshi et al. |
| Citation | Surgery today, 52(11), 1653-1659 https://doi.org/10.1007/s00595-022-02497-5 |
| Issue Date | 2022-11-01 |
| Doc URL | https://hdl.handle.net/2115/90683 |
| Rights | This version of the article has been accepted for publication, after peer review (when applicable) and is subject to Springer Nature's AM terms of use, but is not the Version of Record and does not reflect post-acceptance improvements, or any corrections. The Version of Record is available online at: http://dx.doi.org/10.1007/s00595-022-02497-5 |
| Type | journal article |
| File Information | Surg Today s00595-022-02497-5.pdf |



1 **Title page**

2 **Original Article**

3 **Title:** Tele-assessment of bandwidth limitation for remote robotics surgery

4

5 **All Authors**

6 Yuma Ebihara¹⁾²⁾, Eiji Oki¹⁾³⁾ (co-first author), Satoshi Hirano¹⁾²⁾, Hironobu Takano²⁾, Mitsuhiko Ota³⁾, Hajime

7 Morohashi¹⁾⁴⁾, Kenichi Hakamada¹⁾⁴⁾, Shigeo Urushidani⁵⁾, Masaki Mori¹⁾⁶⁾

8

9 **Institute**

10 1) Committee for Promotion of Remote Surgery Implementation, Japan Surgical Society, Tokyo, Japan

11 2) Department of Gastroenterological Surgery II, Hokkaido University Faculty of Medicine, Sapporo,

12 Japan

13 3) Department of Surgery and Science, Kyushu University, Fukuoka, Japan

14 4) Department of Gastroenterological Surgery, Hirosaki University Graduate School of Medicine,

15 Hirosaki, Japan

16 5) The National Institute of Informatics, Tokyo, Japan

17 6) Tokai University School of Medicine, Isehara, Japan

18

1 **Correspondence author**

2 Satoshi Hirano, MD, PhD

3 Department of Gastroenterological Surgery II, Hokkaido University Faculty of Medicine.

4 North 15 West 7, Kita-ku, Sapporo 0608638, Hokkaido, Japan

5 Tel: +81 11 706 7714 Fax: +81 11 706 7158

6 Email: satto@med.hokudai.ac.jp

7

8 **Short running head:** Tele-assessment of bandwidth limitation for RRS

9

10 **Keywords**

11 robotic surgery, remote robotics surgery, packet loss, communication delay

12

13

14

15

1 **Abstract**

2 **Purpose**

3 This study investigated the communication bandwidth (CB) limitation for remote robotics surgery
4 (RRS) using hinotori™ (Medicaroid, Kobe, Japan).

5 **Methods**

6 The operation rooms of the Hokkaido University Hospital and Kyushu University Hospital were
7 connected using the Science Information NETwork (SINET). The minimum required CB for the RRS was
8 verified by decreasing the CB from 500 to 100 Mbps. Ten surgeons were tested on the task (intracorporeal
9 suturing) at different levels of video compression (VC) amounts (VC1: 120 Mbps, VC2: 40 Mbps, VC3:
10 20 Mbps) with the minimum required CB and assessed based on the task completion time, Global
11 Evaluative Assessment of Robotic Skills (GEARS), and System and Piper Fatigue Scale-12 (PFS-12).

12 **Results**

13 Packet loss was observed at 3–7% and image degradation was observed at 145 Mbps CB. The task
14 performance with VC1 was significantly worse than that with VC2 and VC3 regarding task completion
15 time (VC1 vs. VC2, P=0.032; VC1 vs. VC3, P=0.032), GEARS (VC1 vs. VC2; P=0.029, VC1 vs. VC3;
16 P=0.031), and PFS-12 (VC1 vs. VC2; P=0.032, VC1 vs. VC3; P=0.032) with 145 Mbps.

17 **Conclusion**

18 We concluded that RRS using hinotori™ requires a CB \geq 150 Mbps; when there is insufficient CB,

1 RRS can be continued by compressing the image.

2

3

4

1 **Text**

2 **Introduction**

3 In recent years, the development of high-speed, high-capacity communication technology using
4 optical fiber and 5th generation mobile communication systems (5G), as well as the development of new
5 surgical robots, has made remote surgery a reality [1]. One of the advantages of remote robotics surgery
6 (RRS) is that it can reduce the physical, mental, and financial burden on patients and surgeons by
7 reducing their travel requirements. However, there are still many problems to be solved to implement
8 RRS in society, and one of them is the establishment of a stable communication environment. The
9 occurrence of communication delays or significant packet loss during surgery leads to the distribution of
10 images and inadequate robot functions, which are major obstacles to safe surgery [2-5]. To avoid this, it is
11 essential to determine the communication bandwidth (CB) required for safe and stable telecommunication
12 according to the amount of video data and operation data for each surgical robot. The purpose of this
13 study was to determine the required CB for RRS using hinotori™, a novel surgical robot made in Japan.
14 Setting the required CB is essential to ensure future implementation.

15

16 **Materials and methods**

17 The minimum required CB for RRS using hinotori™ was verified by gradually decreasing the CB
18 from 500 to 100Mbps. We measured the communication round-trip time (RTT; the time in milliseconds

1 from the time the switch on the surgeon cockpit side sends a request to the time the response is received
2 from the switch on the operation unit side), jitter (variation in latency of packet flow), and packet loss (the
3 fraction of the total transmitted packets that did not arrive at the receiver) for each CB. Ten skilled
4 surgeons including 5 gastroenterological surgeon, 2 urologist, 2 gynecologist and a thoracic surgeon were
5 participated in this experiment. They all had sufficient experience in laparoscopic surgery, and experience
6 of robotic surgery.

7 After we found the minimum required bandwidth, the participants were tested on a standard task
8 (intracorporeal suturing) based on the Fundamentals of Laparoscopic Surgery (FLS) curriculum [6] using
9 different video compression (VC; the process of reducing the total number of bits needed to represent a
10 given image or video sequence) amounts (VC1: 120 Mbps, VC2: 40 Mbps, VC3: 20 Mbps) with the
11 minimum required bandwidth. We measured the RTT, jitter, packet loss for the VC amount, task
12 completion time, and robotic surgical skill using the Global Evaluative Assessment of Robotic Skills
13 (GEARS); subjective evaluation of the surgeon was validated using the System and Piper Fatigue Scale-
14 12 (PFS-12).

15

16 (1) Network connections

17 The operation rooms of Hokkaido University Hospital and Kyushu University Hospital were
18 connected by SINET5 (Science Information NETWORK) [7] (Fig. 1). SINET5 is a non-commercial science

1 information network designed and operated by the National Institute of Informatics and provides a nation-
2 wide 100-Gbps backbone for about 1,000 universities and research institutes throughout Japan. For this
3 investigation a virtual private communication circuit was established between the two hospitals along the
4 Japan Sea side, and its circuit distance was about 2,000km on a map basis and about 2,600 km on an
5 optical-fiber-length basis. The CBs of the circuit were set up in the range of 500Mbps to 100Mbps by
6 specifying the rate limits so as to drop information packets if the usage rate of the circuit exceeds the
7 specified rate limit. Communication information was compressed and decompressed using certain
8 encoder and decoder that is evaluated by Mediaroid (Mediaroid Corporation, Kobe, Japan). The
9 encoders and decoders used in this study employ H.265 [8], which is a high compression technology that
10 enables ultra-short delay video transmission and has been applied to ultra-short delay live broadcasting. A
11 raw video is a sequence of images, its size makes it impractical to store or transfer. VC takes advantage of
12 the fact that the frames in a video sequence are highly correlated in time and reduces spatial and temporal
13 redundancy so that as few bits as possible are used to represent the video sequence. Modern standard
14 video compression algorithms such as H.265 are psycho-visually optimized and compress the video data
15 in such a way that quality and detail reduction is, as far as possible, invisible to human perception. To
16 evaluate the communication delay during RRS, we measured RTT of the network line and the packet loss
17 of image signals. RTT is composed of communication line delay (SINET) (Fig. 2).

18

1 (2) Robot system

2 We used a hinotori™ surgical robot system (Medicaroid Corporation, Kobe, Japan). This is the first
3 made-in-Japan robotic system, which recently (August 2020) received regulatory approval from the
4 Japanese Ministry of Health, Labor, and Welfare. A Karl Storz™ 3D endoscope system (Karl Storz,
5 Tuttlingen, Germany) was installed in the system.

6

7 (3) Task: intracorporeal suturing

8 At least three throws of the suture were made, including one double throw and two single throws.
9 The time was measured starting when the instrument appeared on the monitor and ended when the suture
10 material and needle were cut. The task completion time and results of the technical evaluation using
11 GEARS were recorded [9]. The technical evaluation was conducted by two physicians certified in the
12 endoscopic surgical skill qualification system of the Japan Society for Endoscopic Surgery (JSES) [10].
13 The subjective evaluation of the surgeon was validated using PFS-12 [11].

14

15 (4) Statistical analysis

16 Each test score was compared between groups using the Mann–Whitney U test for continuous
17 variables. Statistical significance was set at $P < 0.05$. Statistical analysis was performed using the JMP®
18 software (SAS Institute Inc., Cary, NC, USA).

1

2 **Results**

3 (1) Minimum required CB for RRS using the hinotori™

4 Figure 3 shows an example of the network communication delay, packet loss, and jitter for each CB (500–
5 300–200–150–145 Mbps). Ten surgeon tried simple task such as ring movement in each CB. At 145 Mbps
6 CB, the packet loss was noticeable (3.0–7.0%), and image degradation was observed (Fig. 4.) However,
7 RTT and jitter did not change (RTT, 30–30.4 ms; jitter, 0–0.35 ms).

8

9 (2) Task: intracorporeal suturing

10 Five surgeon tried simulation of intracorporeal suturing in CB of 145Mbps which was revealed to be the
11 minimum required CB for the robot system in the former experiment. Concerning changes in network
12 communication delay in VC2 and VC3, RTT and jitter did not change (RTT, 30–31.5 ms; jitter, 0–0.6 ms),
13 and no packet loss was observed (Fig. 5). The total amount of communication data (including the robot
14 control signal) under a communication bandwidth of 145 Mbps was 130–155 Mbps for VC1, 50–65 Mbps
15 for VC2, and 35–40 Mbps for VC3 (Fig.6). The intracorporeal suturing completion time (VC1:
16 667.4 ± 56.4 s, VC2: 275.8 ± 73.9 s, and VC3: 236.4 ± 42.5 s) was significantly longer in VC1 compared to
17 those in VC2 and VC3 (VC1 vs. VC2, $P=0.009$; VC1 vs. VC3, $P=0.009$; VC2 vs. VC3, $P=0.209$) (Fig.
18 7a). Regarding the GEARS score (VC1, 17.4 ± 1.7 ; VC2, 26.6 ± 3.4 ; VC3, 27.2 ± 1.5), it was

1 significantly lower in VC1 than in VC2 and VC3 (VC1 vs. VC2, P=0.008; VC1 vs. VC3, P=0.009; VC2
2 vs. VC3, P=0.829) (Fig. 7b). The PFS-12 score (VC1, 98.8±18.1; VC2, 34.4±20.5; VC3, 33.2±28.1) was
3 significantly higher in VC1 than in VC2 and VC3 (VC1 vs. VC2, P=0.009; VC1 vs. VC3, P=0.009; VC2
4 vs. VC3, P=0.917) (Fig. 7c).

5

6 **Discussion**

7 In this study, we set up the Japanese-made surgical robot system, hinotori™, in an operating room
8 2,000 km away from the operator to investigate the feasibility of RRS and confirmed the robot's behavior
9 in an environment where surgery is actually possible. In this SINET connection verification, we confirmed
10 that there was no recognizable communication delay or image degradation at a CB of more than 150 Mbps.
11 Furthermore, it was suggested that image degradation could be avoided by considering the amount of VC,
12 even when the available CB is insufficient.

13 Telemedicine has become an inevitable trend during the development of modern medical technology.
14 Teleconsultation, teliagnosis, mobile wards, remote patient image sharing, remote emergency
15 treatment, image sharing and emergency treatment for stroke, digital operating rooms, and distance
16 education have made considerable progress [12-17]. In particular, the development of RRS has been
17 remarkable. Using the ZEUS robotic system and the Transatlantic Optical Faber Network, Jack
18 Marescaux [18, 19] performed the first clinical remote cholecystectomy. This procedure is also known as

1 Lindbergh surgery and is considered a milestone in telesurgery. Subsequently, 22 telesurgeries were
2 performed at a hospital in North Bay, approximately 400 km north of Hamilton, Canada [20]. Although
3 both surgeries were successful, but the transatlantic connection used an expensive dedicated line (10Mbps
4 CB), while the Canadian clinical case used an Internet Protocol-Virtual Private Network line, a special
5 inter-hospital network developed by the government (15Mbps CB). In the USA, Florida Hospital has
6 successfully performed robot-assisted remote surgery using the Internet. Surgeons in Texas, 1,200 miles
7 away from Florida, remotely controlled a da Vinci robot to operate on a simulated patient via the Internet
8 [21]. In Japan, robotic telesurgical simulation for training was reported by Hashizume et al. [22].
9 Consequently, the underdeveloped information and communication technology was a decisive factor that
10 led to a long hiatus in telesurgery research [23]. The recent development of high-speed, high-capacity
11 communication technology using optical fiber and 5G, as well as the development of new surgical robots,
12 is making remote surgery a reality [24]. The bandwidth of the optical fiber and 5G network were 1 Gbps,
13 which is comparable to the bearing capacity of the Internet and 100 times wider than that of the satellite
14 network [1]. In the future, it is expected that robotic surgery using the Internet will further develop with
15 the evolution of technology.

16 However, there are many problems to be solved in RRS, one of which is the establishment of a stable
17 communication environment. Communication delays during RRS can be a major obstacle to safe surgical
18 procedures [2-5]. In general, regarding the transmission delay, it has been reported that operability

1 decreases when the delay time perceived by the surgeon exceeds 200 ms, errors increase when the delay
2 time exceeds 300 ms [25, 26], and work becomes almost impossible when the delay time exceeds 700 ms
3 [27]. Many reports suggest that the delay time should be less than 200 ms, ideally less than 100 ms, for
4 normal robot operation [28, 29].

5 In this study, it was possible to operate with minimal delay (<30 ms) for all CBs; however, image
6 degradation was observed in the 145 Mbps CB. When robot control signals and audio signals were
7 included in addition to the image signals, the traffic from all the signals exceeded 145 Mbps, and image
8 degradation was observed. Because of the degraded images, the task completion time increased, and the
9 surgeon's fatigue increased. The reason why image degradation rather than image delay occurred when
10 reducing CB was thought to be the adoption of traffic policing, which cuts off some of the traffic that
11 exceed the rate limit on SINET lines. At 145 Mbps, by changing the VC amount (VC 2: 40 Mbps, VC 3:
12 20 Mbps), image degradation disappeared at the same CB, and we could not discern any decrease in
13 image quality. In addition to image degradation, information and communication processing technology
14 to compress and decompress transmission data is also important. The largest volume of transmission
15 signals in the RRS is the video signal, which is strongly affected by the CB. Therefore, information and
16 compression processing technologies are essential; however, the compression and decompression
17 processes also cause delays. Because there is a trade-off between the compression ratio and time required
18 for compression and decompression, it is necessary to develop encoders and decoders that achieve high

1 compression and low delay. In this study, excessive image capacity load might cause image degradation,
2 and the amount of VC needed to be adjusted as a countermeasure.

3 In this study, despite the long communication distance of approximately 4000 km round trip, we
4 were able to communicate 3D 2K images without image degradation with an RTT of 30 ms which hardly
5 affected the surgeon's performance. Furthermore, even with a CB of 145 Mbps, we were able to perform
6 the task without any image degradation or delay using image compression technology. In the future, the
7 limitations of CB may be overcome by the development of encoders, decoders, and 5G communication
8 technologies that enable low-latency transmission of high-precision images, such as 8K and 16K.

9 In this study, we demonstrated that hinotoriTM can be used in commercial communications by
10 selecting a bandwidth type of service of more than 150 Mbps. Currently, there are two types of
11 commercial communication networks, open and closed networks, which differ in their degree of security
12 assurance, communication quality, and cost. In RRS, it is important to select a communication network
13 based on the premise of sufficient communication quality and security while considering economic
14 efficiency. For future clinical applications of RRS, it would be desirable to develop guidelines for optimal
15 communication systems focusing on safety, ethics, and costs.

16 In recent years, 5G communication technology has been reported to have advantages such as high
17 speed and large capacity communication, high mobility, multiple connections, and wide bandwidth, which
18 will be beneficial for robots that require a wide bandwidth for high-quality transmission, such as 4K/8K

1 video [1]. The 5G network has many advantages, such as wider bandwidth and lower latency time than
2 the previous 4G network. Furthermore, unlike the wired Internet, the 5G wireless network has high
3 mobility and eliminates the regional restriction of special network cables. Therefore, RSS is expected to
4 be realized in isolated islands and disaster areas where it is difficult to lay wired Internet cables. In
5 addition, surgeries performed during the current coronavirus disease 2019 pandemic era need to avoid
6 infection crises due to the flow of people. In this situation, RSS using 5G is expected to be able to support
7 remote surgeries in regional hospitals throughout Japan and help train young surgeons.

8 This study has several limitations. Because of the limited duration of the experiment, the number of
9 tasks was small, and the time to practice the robot operation was short. The image quality was evaluated
10 based on the surgeon's impression, and no objective data analysis was conducted. In the future, remote
11 surgery using high-precision images is possible, and a universal image evaluation method is necessary.

12

13 **Conclusion**

14 RRS using the novel hinotoriTM surgical robot system can be performed safely if the CB is ≥ 150
15 Mbps. RRS can be implemented in society using currently available commercial communication
16 networks.

17

18 **Acknowledgments**

1 This study was conducted as part of the Advanced Telemedicine Network Research Project of the
2 Japan Agency for Medical Research and Development (AMED), and we are grateful for the financial
3 support. We thank all physicians including gastroenterological and thoracic surgeon, urologist,
4 gynecologist and engineers participating in this study. We would also like to express our deepest
5 gratitude to the Mediaroid Corporation for their cooperation in the experiments.

6

7 **Disclosure**

8 This work was supported by a grant from the Japan Agency for Medical Research and Development
9 (AMED) (Grant Number 21hs0122001h0002).

10

11

12

13

14

15

16

17

18

1

2 **References**

3 1. Zheng J, Wang Y, Zhang J, Guo W, Yang X, Luo L et al. 5G ultra-remote robot-assisted
4 laparoscopic surgery in China. *Surg Endosc.* 2020 Nov;34(11):5172–80. doi: 10.1007/s00464-020-07823-
5 x. [Epub 2020 Jul 22]. PMID: 32700149.

6 2. Sterbis JR, Hanly EJ, Herman BC, Marohn MR, Broderick TJ, Shih SP et al. Transcontinental
7 telesurgical nephrectomy using the da Vinci robot in a porcine model. *Urology.* 2008 May;71(5):971–3.
8 doi: 10.1016/j.urology.2007.11.027. [Epub 2008 Mar 4]. PMID: 18295861

9 3. Nguan C, Miller B, Patel R, Luke PP, Schlachta CM. Pre-clinical remote telesurgery trial of a
10 da Vinci telesurgery prototype. *Int J Med Robot.* 2008 Dec;4(4):304–9. doi: 10.1002/rcs.210, PMID:
11 18803341

12 4. Raison N, Khan MS, Challacombe B. Telemedicine in surgery: what are the opportunities and
13 hurdles to realising the potential? *Curr Urol Rep.* 2015 Jul;16(7):43. doi: 10.1007/s11934-015-0522-x,
14 PMID: 26025497

15 5. Korte C, Nair SS, Nistor V, Low TP, Doarn CR, Schaffner G. Determining the threshold of
16 time-delay for teleoperation accuracy and efficiency in relation to telesurgery. *Telemed J E Health.* 2014
17 Dec;20(12):1078–86. doi: 10.1089/tmj.2013.0367, PMID: 25290465

18 6. Okraïneç A, Soper NJ, Swanstrom LL, Fried GM. Trends and results of the first 5 years of

- 1 Fundamentals of Laparoscopic Surgery (FLS) certification testing. *Surg Endosc.* 2011 Apr;25(4):1192–8.
2 doi: 10.1007/s00464-010-1343-0. [Epub 2010 Sep 25]. PMID: 20872021
- 3 7. T. Kurimoto, S. Urushidani, H. Yamada, K. Yamanaka, M. Nakamura, S. Abe. et al., SINET5:
4 A low-latency and high-bandwidth backbone network for SDN/NFV Era. *IEEE International Conference*
5 *on Communications (ICC)*; 2017. <https://doi.org/10.1109/ICC.2017.7996843>.
- 6 8. Uhrina M, Holesova A, Bienik J, Sevcik L. Impact of scene content on high resolution video
7 quality. *Sensors (Basel)*. 2021 Apr 19;21(8):2872. doi: 10.3390/s21082872, PMID: 33921877, PMCID:
8 PMC8073500
- 9 9. Aghazadeh MA, Jayaratna IS, Hung AJ, Pan MM, Desai MM, Gill IS et al. External validation
10 of Global Evaluative Assessment of Robotic Skills (GEARS). *Surg Endosc.* 2015 Nov;29(11):3261–6.
11 doi: 10.1007/s00464-015-4070-8. [Epub 2015 Jan 22]. PMID: 25609318
- 12 10. Japanese Society for Endoscopic Surgery. Guidelines for the management of endoscopic
13 surgery. Tokyo: Japanese Society for Endoscopic Surgery; 2014
- 14 11. Reeve BB, Stover AM, Alfano CM, Smith AW, Ballard-Barbash R, Bernstein L et al. The Piper
15 Fatigue Scale-12 (PFS-12): psychometric findings and item reduction in a cohort of breast cancer
16 survivors. *Breast Cancer Res Treat.* 2012 Nov;136(1):9–20. doi: 10.1007/s10549-012-2212-4. [Epub
17 2012 Aug 30]. PMID: 22933027, PMCID: PMC3739964
- 18 12. Martinez AW, Phillips ST, Carrilho E, Thomas SW 3rd, Sindi H, Whitesides GM. Simple

- 1 telemedicine for developing regions: camera phones and paper-based microfluidic devices for real-time,
2 off-site diagnosis. *Anal Chem.* 2008 May 15;80(10):3699–707. doi: 10.1021/ac800112r. [Epub 2008 Apr
3 11]. PMID: 18407617, PMCID: PMC3761971
- 4 13. Weinstein RS, Lopez AM, Joseph BA, Erps KA, Holcomb M, Barker GP et al. Telemedicine,
5 telehealth, and mobile health applications that work: opportunities and barriers. *Am J Med.* 2014
6 Mar;127(3):183–7. doi: 10.1016/j.amjmed.2013.09.032. [Epub 2013 Oct 29]. PMID: 24384059
- 7 14. Kim DK, Yoo SK, Park IC, Choa M, Bae KY, Kim YD et al. A mobile telemedicine system for
8 remote consultation in cases of acute stroke. *J Telemed Telecare.* 2009;15(2):102–7. doi:
9 10.1258/jtt.2008.080713, PMID: 19246612
- 10 15. Bolsi A, Lomax AJ, Pedroni E, Goitein G, Hug E. Experiences at the Paul Scherrer Institute
11 with a remote patient positioning procedure for high-throughput proton radiation therapy. *Int J Radiat
12 Oncol Biol Phys.* 2008 Aug 1;71(5):1581–90. doi: 10.1016/j.ijrobp.2008.02.079, PMID: 18640501
- 13 16. Heslop L, Weeding S, Dawson L, Fisher J, Howard A. Implementation issues for mobile-
14 wireless infrastructure and mobile health care computing devices for a hospital ward setting. *J Med Syst.*
15 2010 Aug;34(4):509–18. doi: 10.1007/s10916-009-9264-y. [Epub 2009 Mar 11]. PMID: 20703905
- 16 17. Chan FY, Whitehall J, Hayes L, Taylor A, Soong B, Lessing K et al. Minimum requirements for
17 remote realtime fetal tele-ultrasound consultation. *J Telemed Telecare.* 1999;5(3):171–6. doi:
18 10.1258/1357633991933585, PMID: 10628032

- 1 18. Marescaux J, Leroy J, Gagner M, Rubino F, Mutter D, Vix M et al. Transatlantic robot-assisted
2 telesurgery. *Nature*. 2001 Sep 27;414(6865):379–80. doi: 10.1038/35096636. Erratum in: *Nature*. 2001
3 Dec 13;414(6865):710. PMID: 11574874
- 4 19. Marescaux J, Leroy J, Rubino F, Smith M, Vix M, Simone M et al. Transcontinental robot-
5 assisted remote telesurgery: feasibility and potential applications. *Ann Surg*. 2002 Apr;235(4):487–92.
6 doi: 10.1097/00000658-200204000-00005, PMID: 11923603, PMCID: PMC1422462
- 7 20. Anvari M, McKinley C, Stein H. Establishment of the world's first telerobotic remote surgical
8 service: for provision of advanced laparoscopic surgery in a rural community. *Ann Surg*. 2005
9 Mar;241(3):460–4. doi: 10.1097/01.sla.0000154456.69815.ee, PMID: 15729068, PMCID: PMC1356984
- 10 21. Sterbis JR, Hanly EJ, Herman BC, Marohn MR, Broderick TJ, Shih SP, Harnett B, Doarn C,
11 Schenkman NS. Transcontinental telesurgical nephrectomy using the da Vinci robot in a porcine model.
12 *Urology*. 2008 May;71(5):971-3. doi: 10.1016/j.urology.2007.11.027. Epub 2008 Mar 4. PMID:
13 18295861.
- 14 22. Suzuki S, Suzuki N, Hayashibe M, Hattori A, Konishi K, Kakeji Y et al. Tele-surgical
15 simulation system for training in the use of da Vinci surgery. *Stud Health Technol Inform*. 2005;111:543–
16 8. PMID: 15718794
- 17 23. Choi PJ, Oskouian RJ, Tubbs RS. Telesurgery: Past, Present, and Future. *Cureus*. 2018 May
18 31;10(5):e2716. doi: 10.7759/cureus.2716. PMID: 30079282; PMCID: PMC6067812.

- 1 24. Hakamada K, Mori M. The changing surgical scene: From the days of Billroth to the upcoming
2 future of artificial intelligence and telerobotic surgery. *Ann Gastroenterol Surg.* 2021 May 29;5(3):268-
3 269. doi: 10.1002/ags3.12466. PMID: 34095715; PMCID: PMC8164454.
- 4 25. Kim T, Zimmerman PM, Wade MJ, Weiss CA 3rd. The effect of delayed visual feedback on
5 telerobotic surgery. *Surg Endosc.* 2005 May;19(5):683–6. doi: 10.1007/s00464-004-8926-6. [Epub 2005
6 Mar 23]. PMID: 15776211
- 7 26. Xu S, Perez M, Yang K, Perrenot C, Felblinger J, Hubert J. Effect of latency training on
8 surgical performance in simulated robotic telesurgery procedures. *Int J Med Robot.* 2015 Sep;11(3):290–
9 5. doi: 10.1002/rcs.1623. [Epub 2014 Oct 19]. PMID: 25328078
- 10 27. Perez M, Xu S, Chauhan S, Tanaka A, Simpson K, Abdul-Muhsin H et al. Impact of delay on
11 telesurgical performance: study on the robotic simulator dV-Trainer. *Int J Comput Assist Radiol Surg.*
12 2016 Apr;11(4):581–7. doi: 10.1007/s11548-015-1306-y. [Epub 2015 Oct 8]. PMID: 26450105
- 13 28. Wirz R, Torres LG, Swaney PJ, Gilbert H, Alterovitz R, Webster RJ 3rd et al. An experimental
14 feasibility study on robotic endonasal telesurgery. *Neurosurgery.* 2015 Apr;76(4):479–84; discussion 484.
15 doi: 10.1227/NEU.0000000000000623, PMID: 25599203, PMCID: PMC4366329
- 16 29. Xu S, Perez M, Yang K, Perrenot C, Felblinger J, Hubert J. Determination of the latency effects
17 on surgical performance and the acceptable latency levels in telesurgery using the dV-Trainer(®)
18 simulator. *Surg Endosc.* 2014 Sep;28(9):2569–76. doi: 10.1007/s00464-014-3504-z. [Epub 2014 Mar 27].

1 PMID: 24671353

2 **Figure legends**

3

4 **Fig. 1** Schema of network connection for remote robotics surgery

5 The operation rooms of Hokkaido University Hospital and Kyushu University Hospital (network
6 communication distance of nearly 2,000 km) were connected by SINET.

7 SINET; Science Information NETwork, HUH; Hokkaido University Hospital, KUH; Kyushu University
8 Hospital

9

10 **Fig. 2** Network system

11 Round trip time (RTT) is composed of communication line delay (SINET). SINET; Science
12 Information NETwork

13

14 **Fig. 3** The packet loss and jitter for communication bandwidths of 500 Mbps, 300 Mbps, 200 Mbps, 150
15 Mbps, and 145 Mbps

16 At 145 Mbps, the packet loss was noticeable (3–7 %); however, the round-trip time (RTT) and jitter
17 did not change (RTT, 30–30.4 ms; jitter, 0–0.35 ms)

18

1 **Fig. 4** Operation image from 145-Mbps communication bandwidth

2 At 145 Mbps, image degradation was observed

3

4 **Fig. 5** Comparison of round-trip time (RTT), packet loss, and jitter depending on the video compression

5 (VC) amount

6 At VC 1 (120 Mbps), packet loss was between 3% and 7%. At VC 2 (40 Mbps) and VC 3 (20 Mbps),

7 packet loss was not observed. RTT and jitter showed no changes (RTT, 30–31.5 ms, jitter, 0–1.0 ms) for all

8 VC

9

10 **Fig. 6** Total amount of communication data under communication bandwidth of 145 Mbps

11 The total amount of communication data (including the robot control signal) was 130–155 Mbps at

12 video compression (VC) 1 (120 Mbps), 50–65 Mbps at VC 2 (40 Mbps), 35–40 Mbps at VC 3 (20

13 Mbps)

14


15 **Fig. 7** Intracorporeal suturing completion time, and the robotic skill evaluation using the Global Evaluative

16 Assessment of Robotic Skills (GEARS), and the subjective evaluation of the surgeon was validated using

17 the System and Piper Fatigue Scale-12 (PFS-12)


18 a. Intracorporeal suturing completion time: VC1 significantly prolonged the task completion time

- 1 compared to that with VC2 and VC3 (P= 0.009 and P=0.009, respectively). b. GEARS scores with VC1
- 2 were significantly lower than those with VC2 and VC3 (P=0.008 and P=0.009, respectively). c. PFS-12
- 3 scores with VC1 were significantly higher than those with VC2 and VC3 (P= 0.009 and P=0.009,
- 4 respectively).
- 5 VC: video compression (VC1, 120 Mbps; VC2, 40 Mbps; VC3, 20 Mbps)


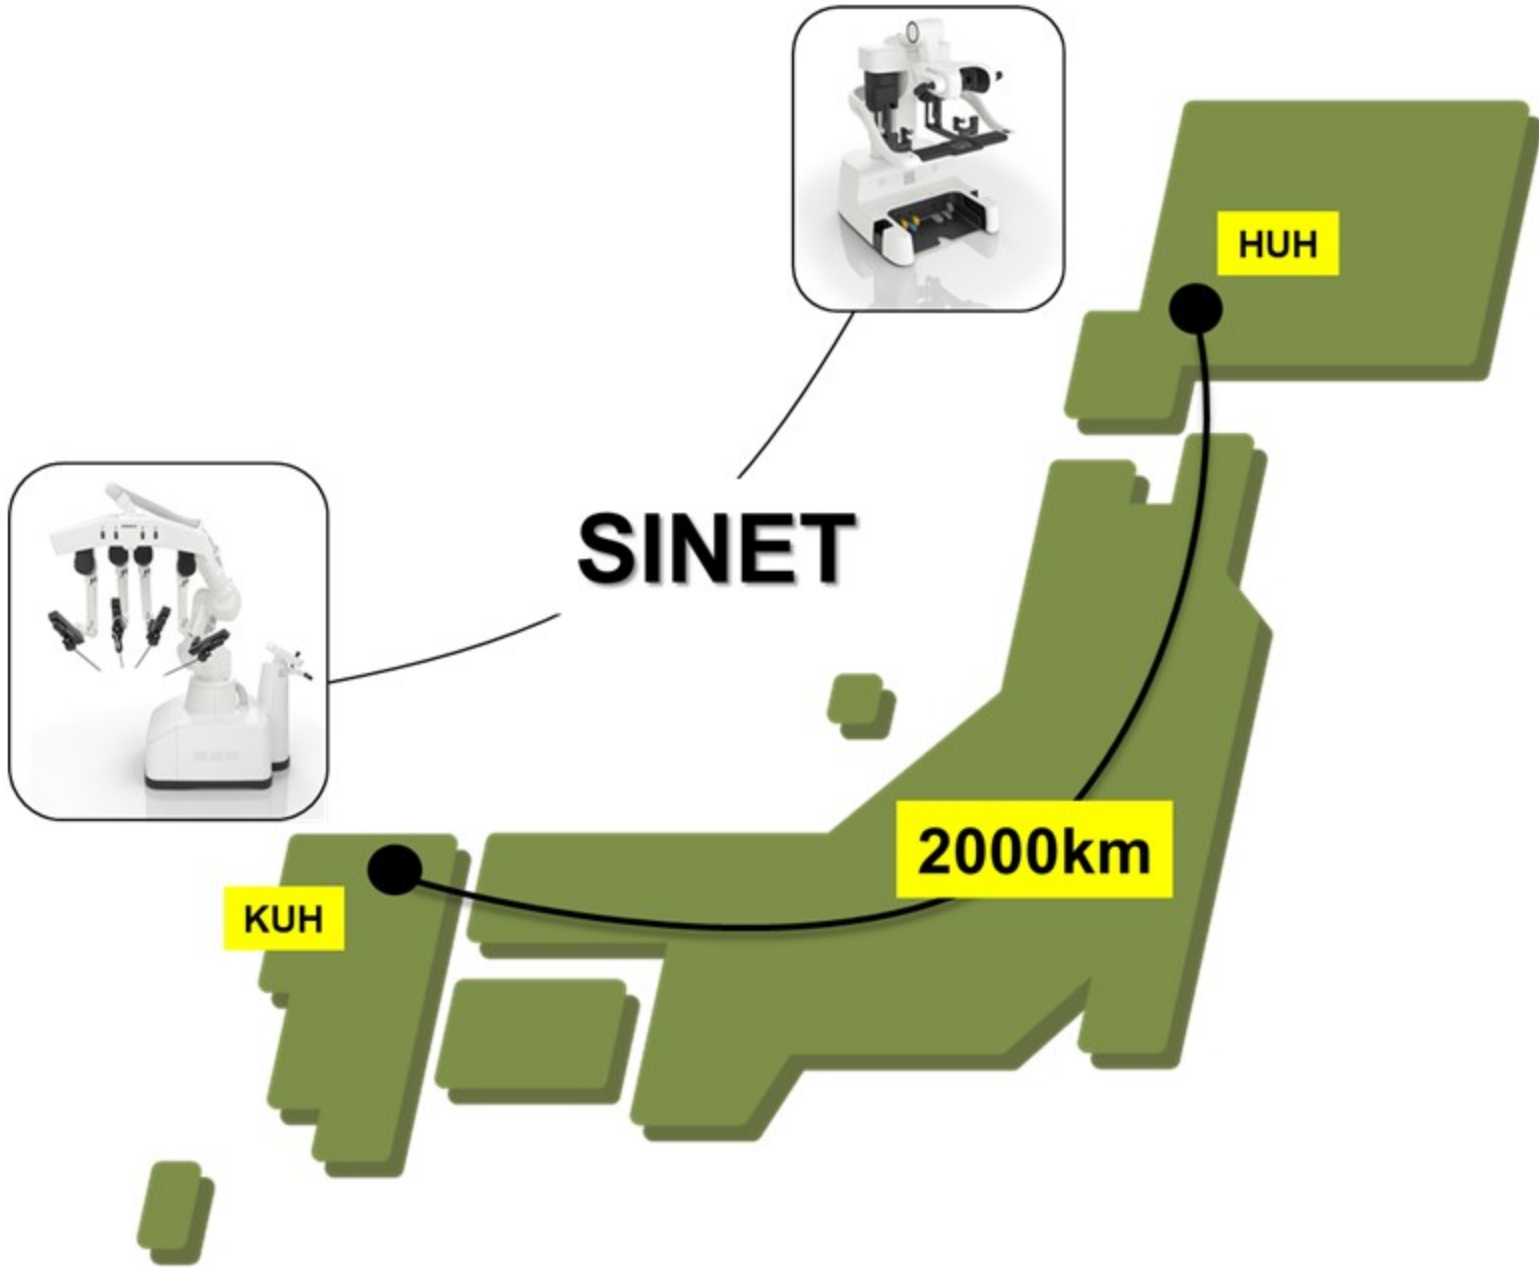







Operation unit

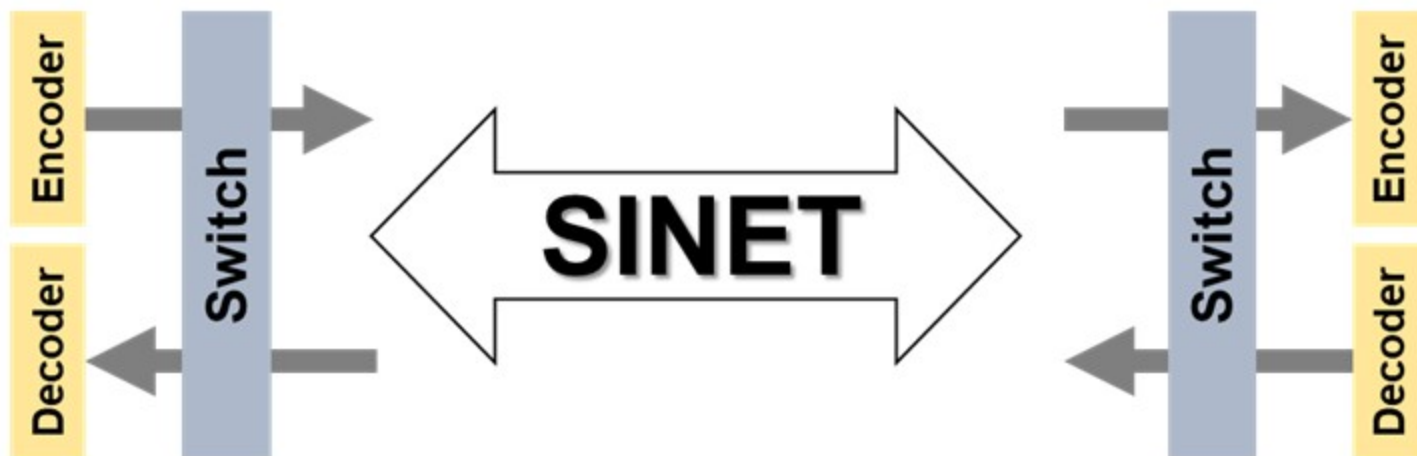

Surgeon cockpit

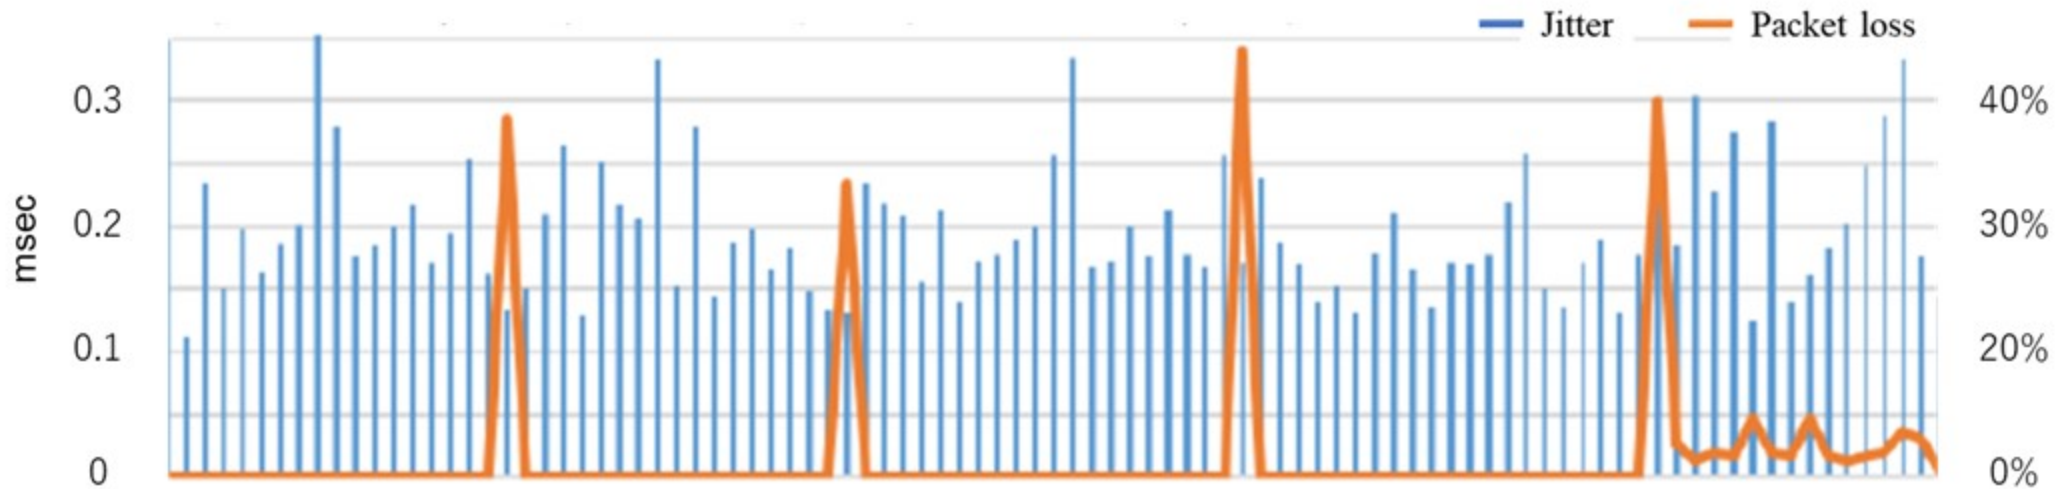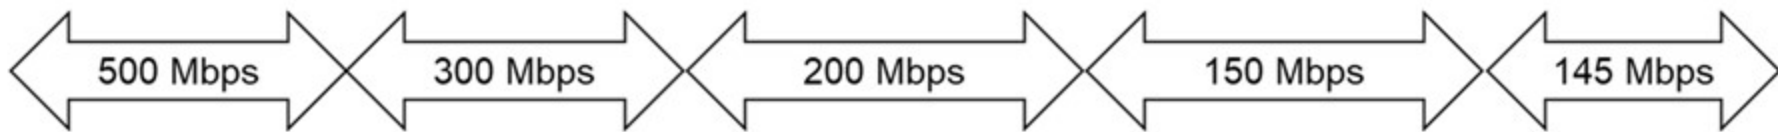



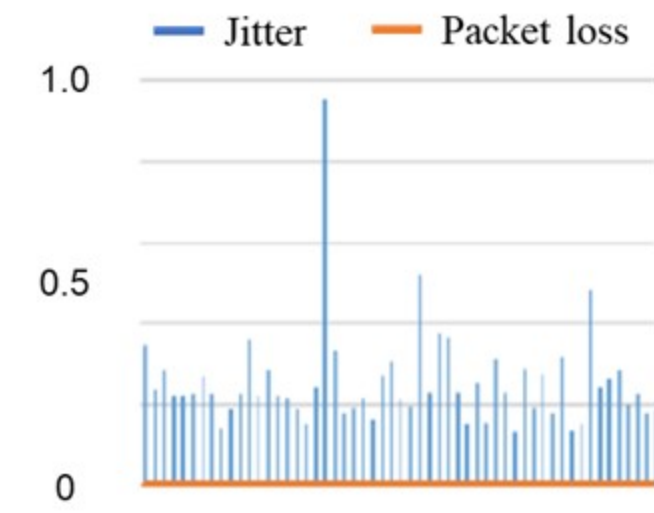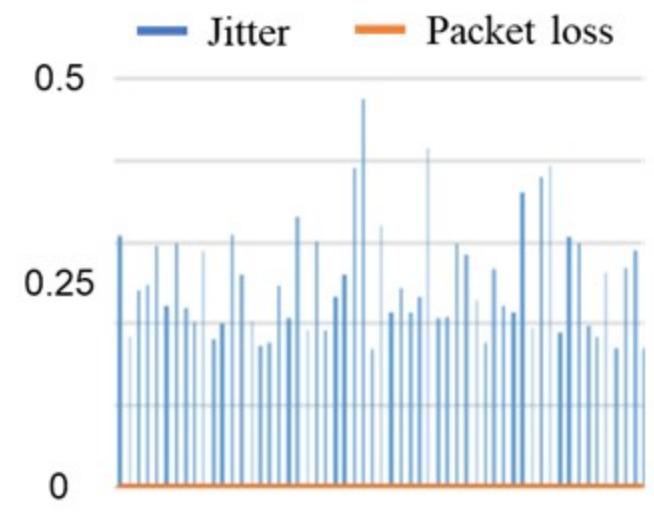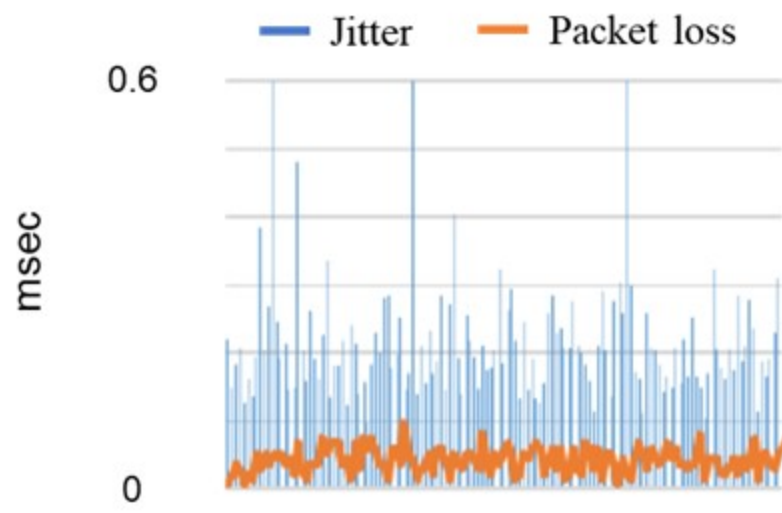

VC 1 (120 Mbps)

VC 2 (40 Mbps)

VC 3 (20 Mbps)

